

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/22/2024

OPERATOR NAME:  
JOHN D BATEHOLTS  
Permit #: 43007  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:13
INTERNAL STANDARD	VERIFIED	07:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:13
BLANK TEST	0.00	07:14
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:14
BLANK TEST	0.00	07:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:16
BLANK TEST	0.00	07:16

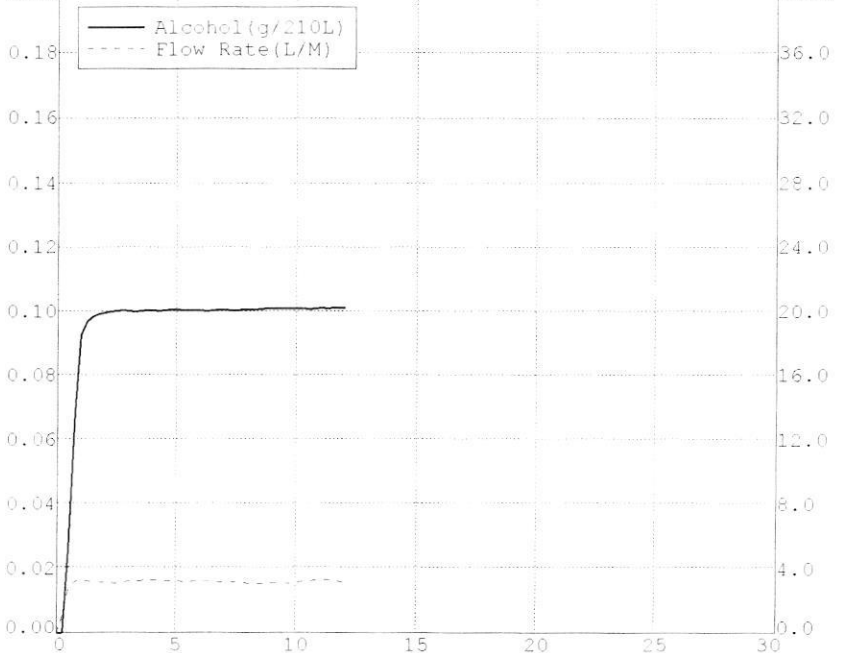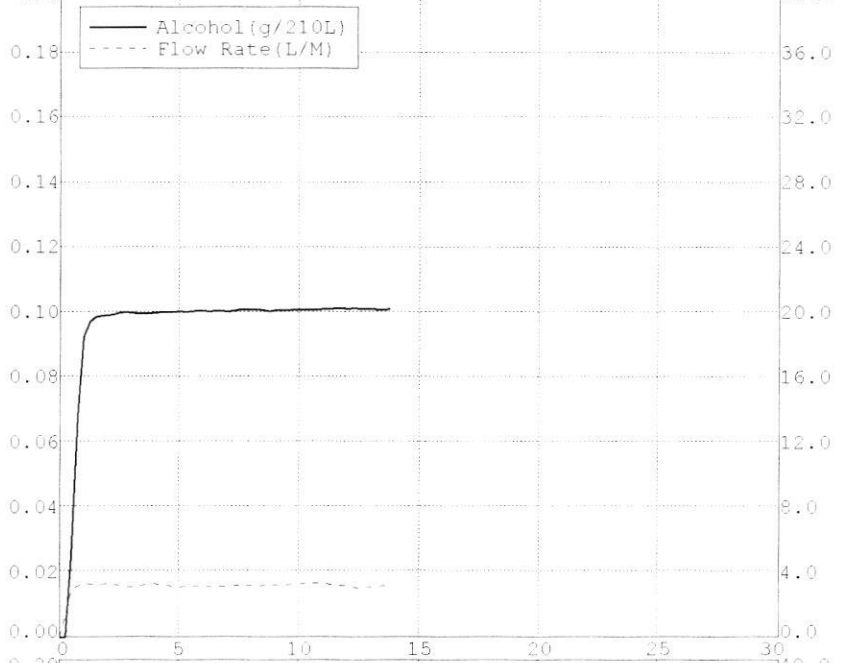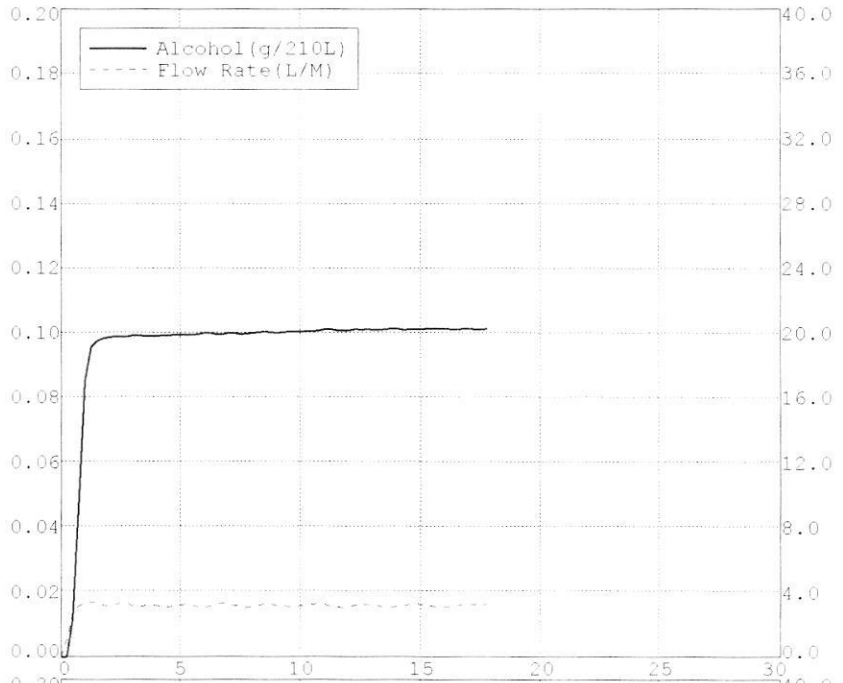

*John D. Bateholts* 714