

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/22/2024

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:25
INTERNAL STANDARD	VERIFIED	06:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:25
BLANK TEST	0.00	06:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:26
BLANK TEST	0.00	06:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:28
BLANK TEST	0.00	06:29

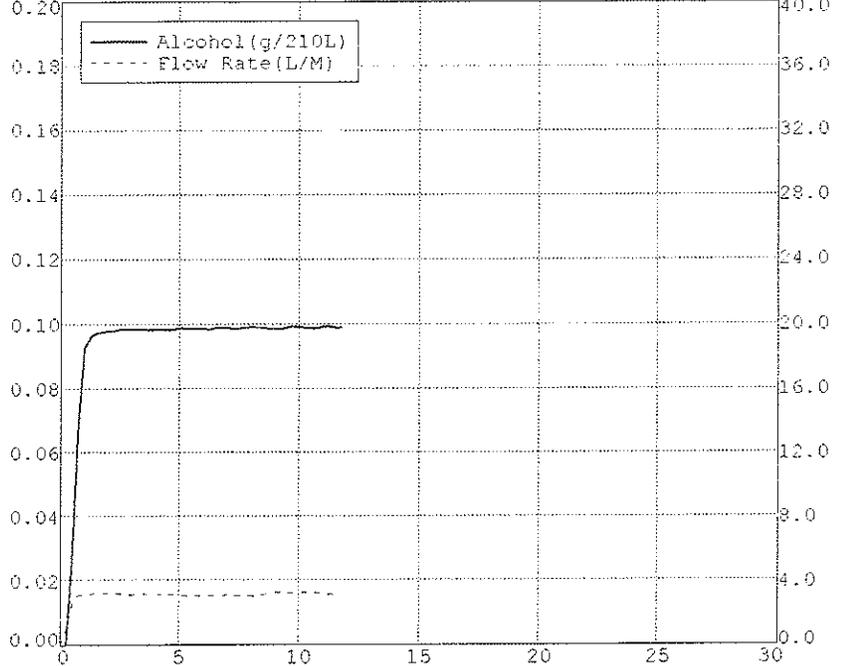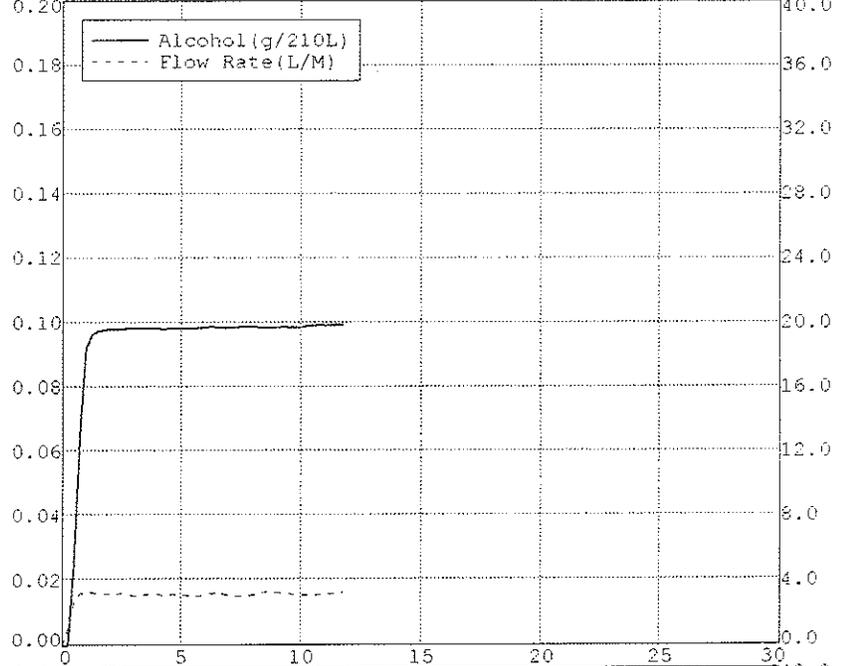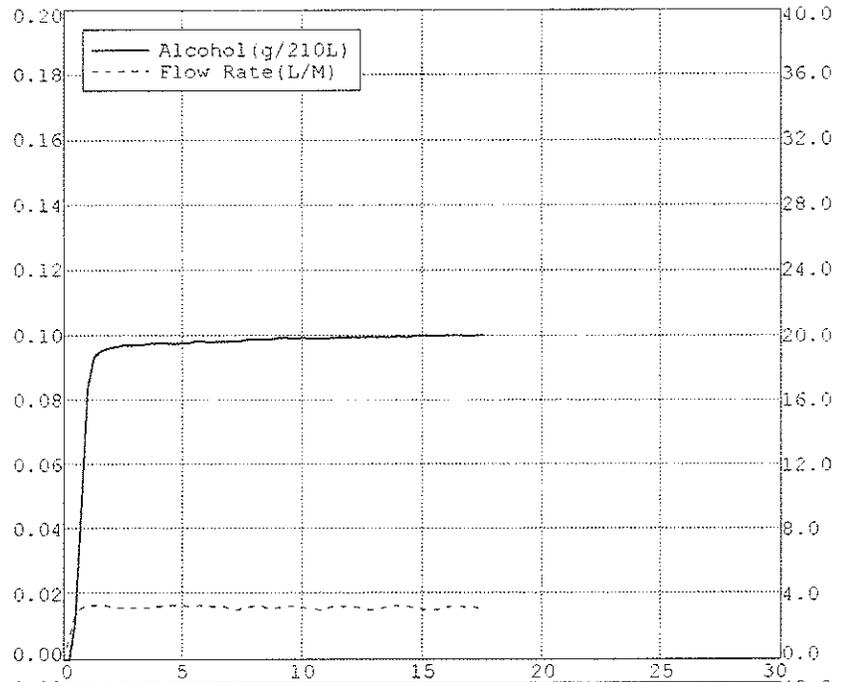

SGT *[Signature]* #157