

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 09/10/2024

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:27
INTERNAL STANDARD	VERIFIED	08:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:27
BLANK TEST	0.00	08:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:28
BLANK TEST	0.00	08:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:30
BLANK TEST	0.00	08:31

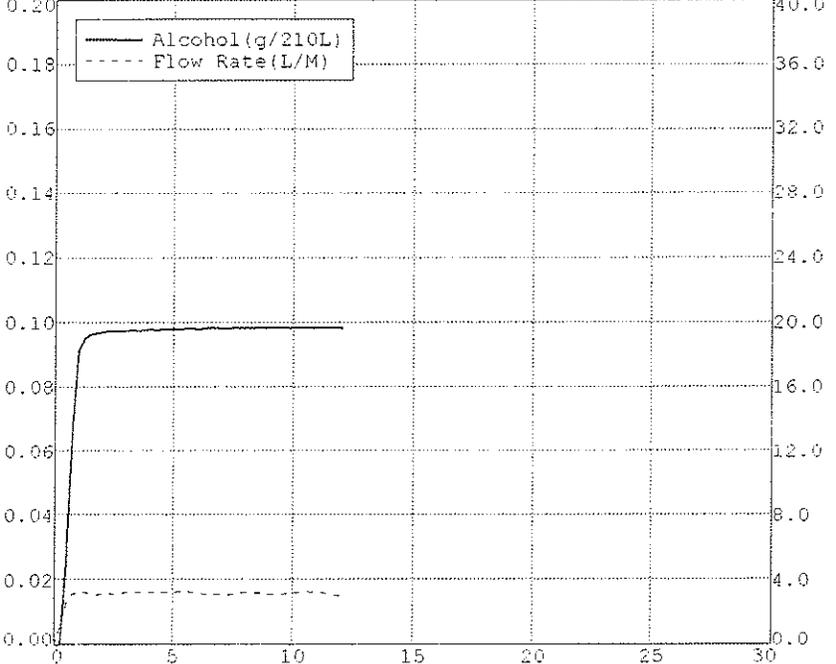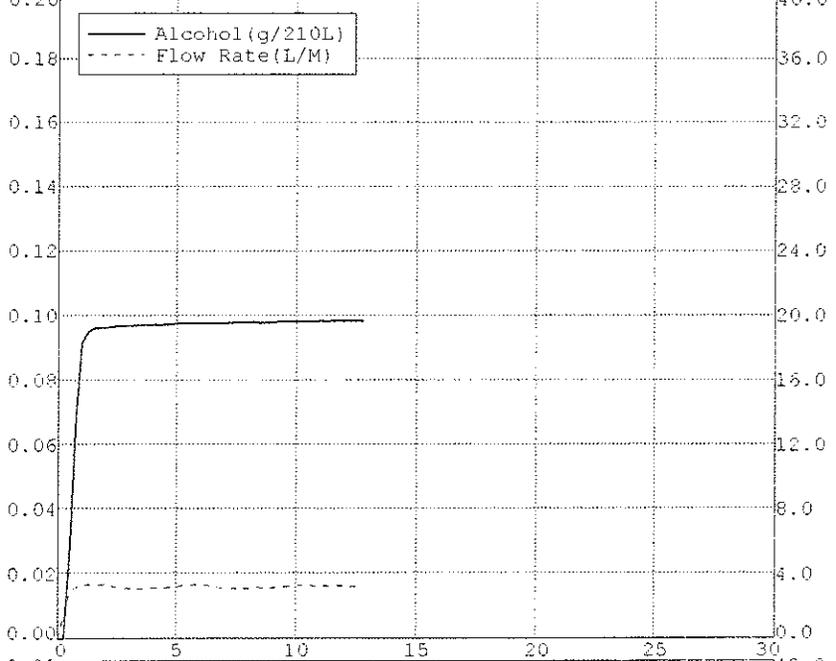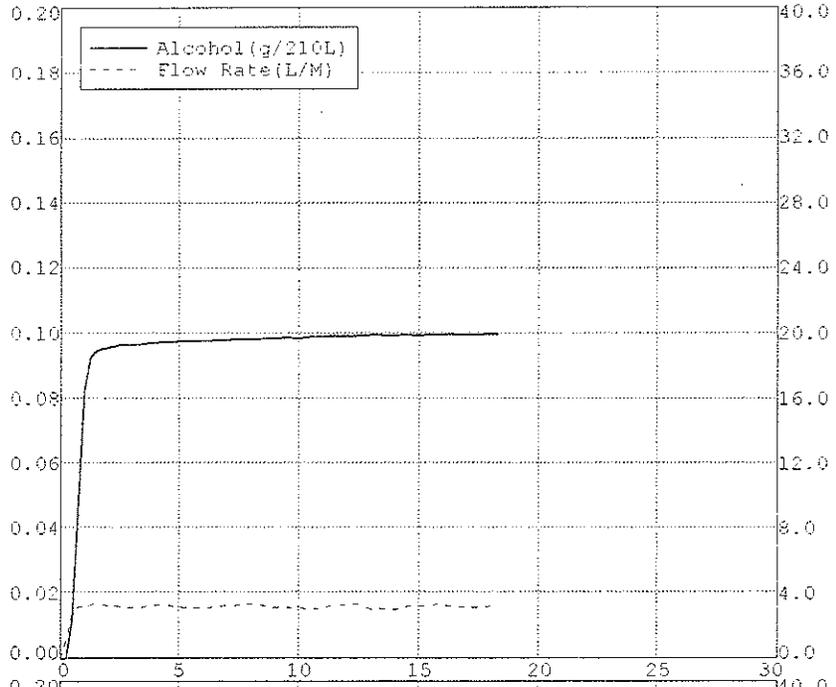

*Charles B. Geisler*