

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/16/2024

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:01
INTERNAL STANDARD	VERIFIED	10:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:02
BLANK TEST	0.00	10:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:03
BLANK TEST	0.00	10:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	10:04
BLANK TEST	0.00	10:05

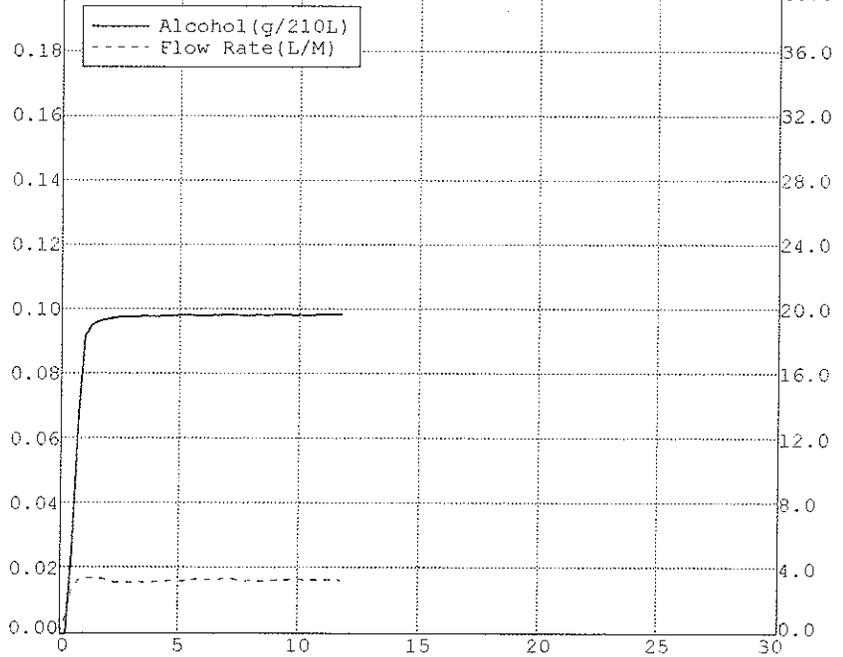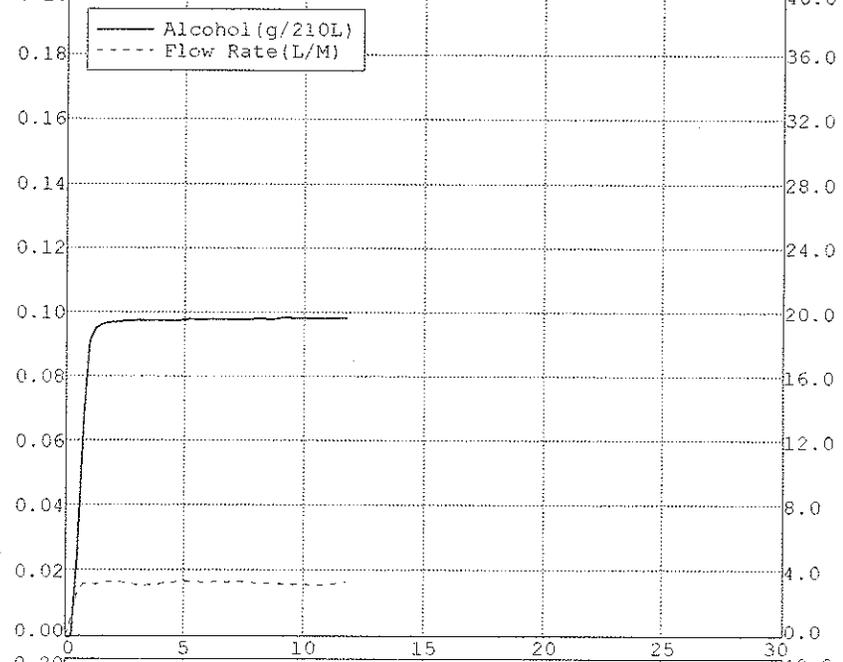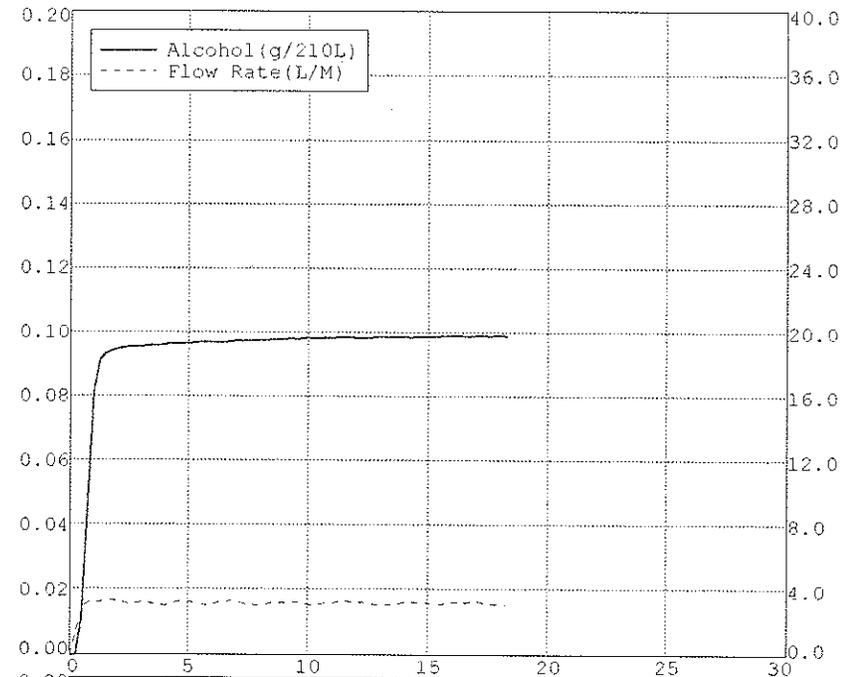

SGT *[Signature]* # 757