

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/02/2025

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:38
INTERNAL STANDARD	VERIFIED	08:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:38
BLANK TEST	0.00	08:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:39
BLANK TEST	0.00	08:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:41
BLANK TEST	0.00	08:41

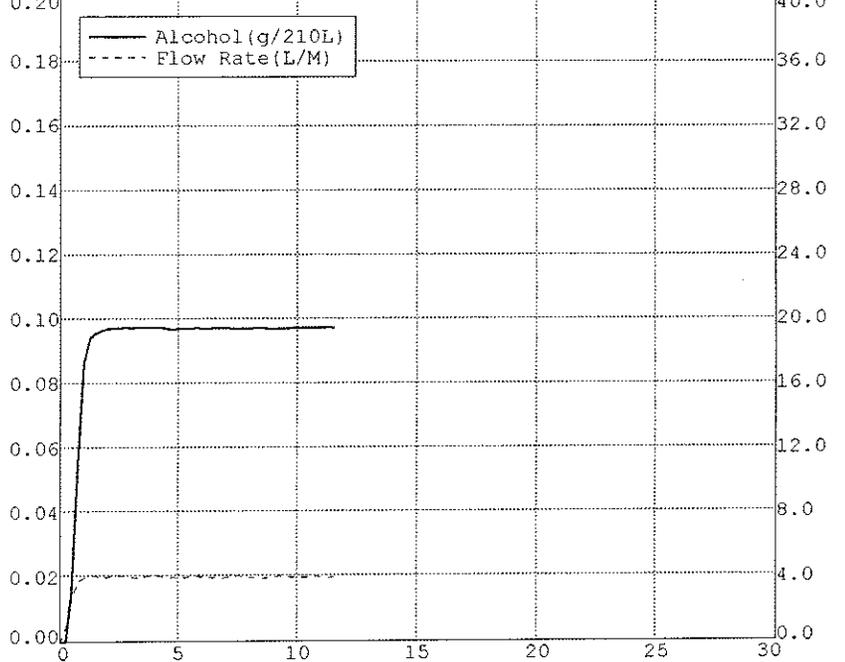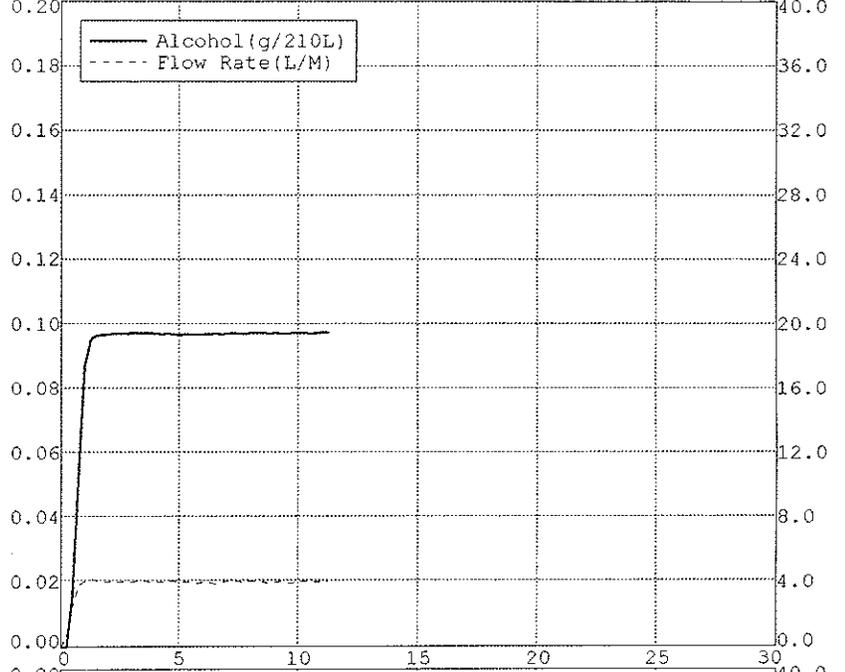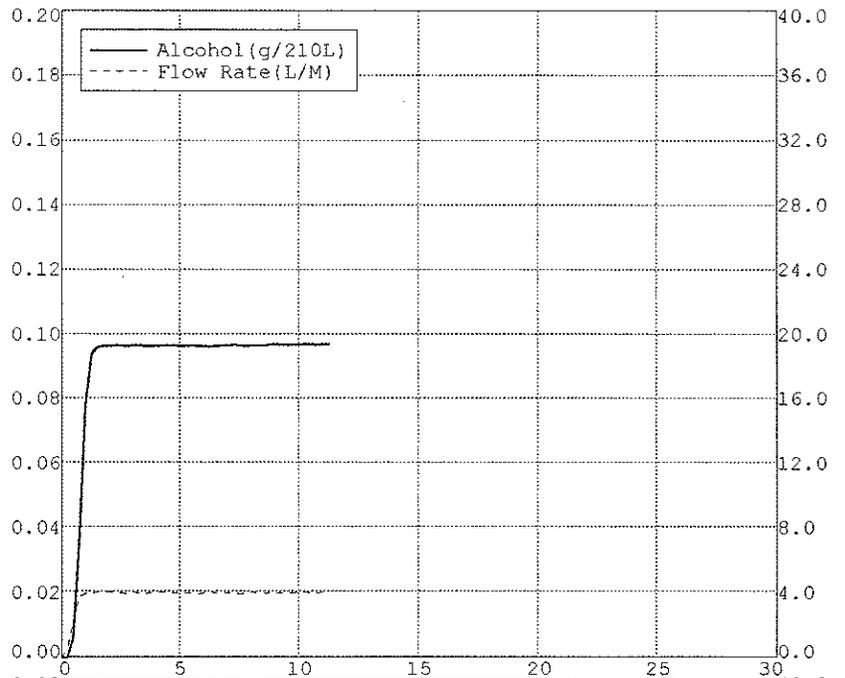

John D Bateholts 0714