

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/24/2025

OPERATOR NAME:  
JOHN D BATEHOLTS  
Permit #: 43007  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:13
INTERNAL STANDARD	VERIFIED	10:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:13
BLANK TEST	0.00	10:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:14
BLANK TEST	0.00	10:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:15
BLANK TEST	0.00	10:16

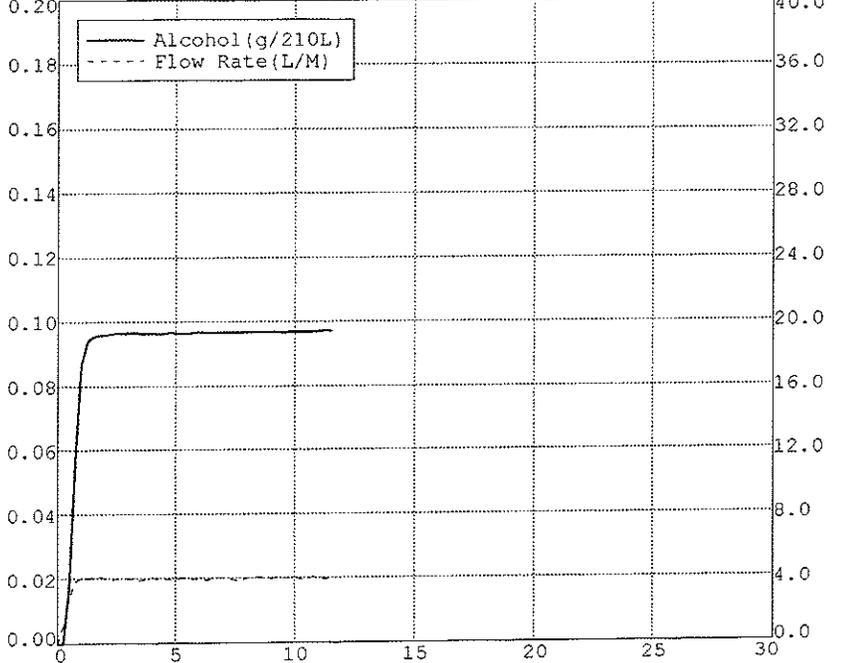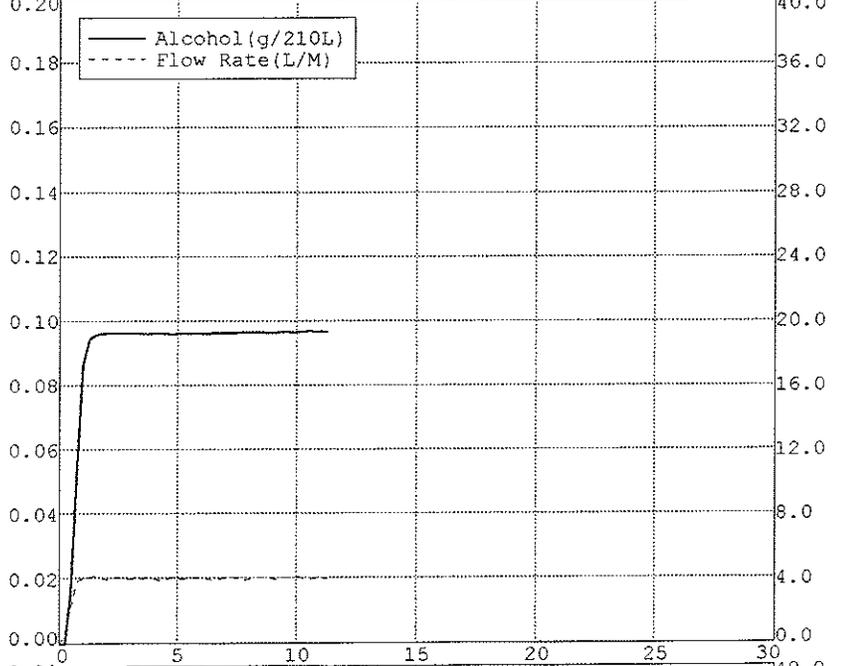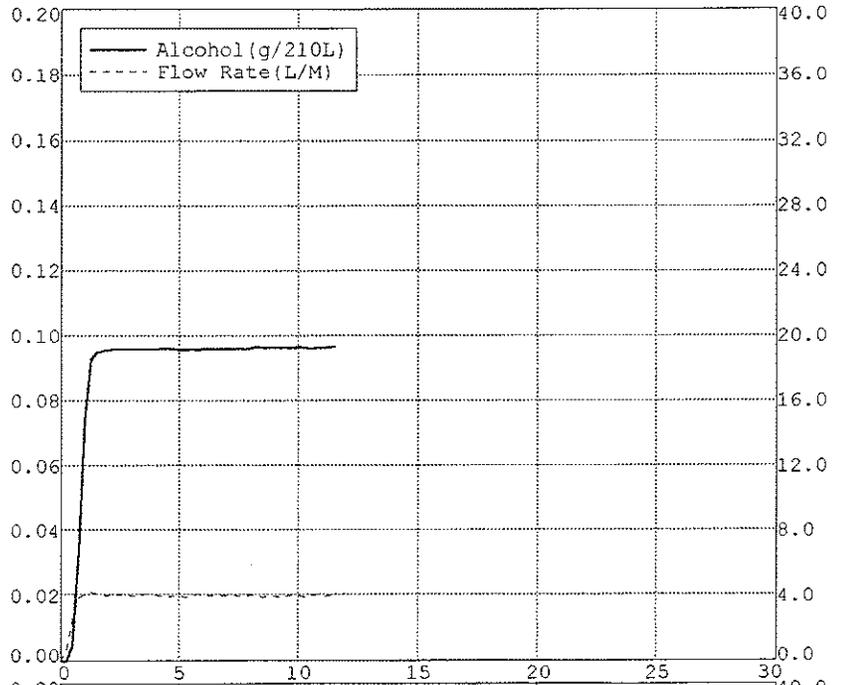

*John D Bateholts #714*