

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/21/2025

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:56
INTERNAL STANDARD	VERIFIED	02:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:56
BLANK TEST	0.00	02:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:57
BLANK TEST	0.00	02:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:59
BLANK TEST	0.00	02:59

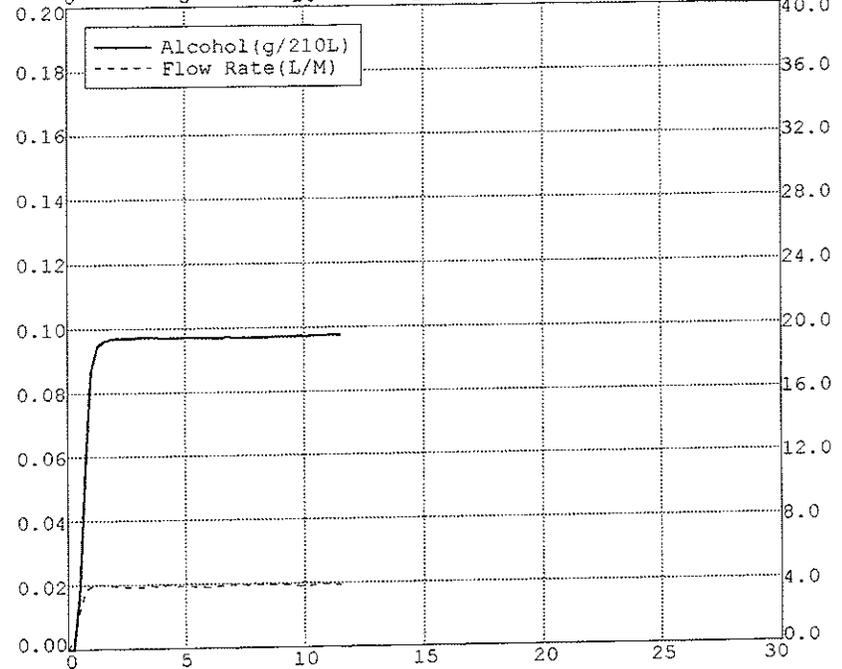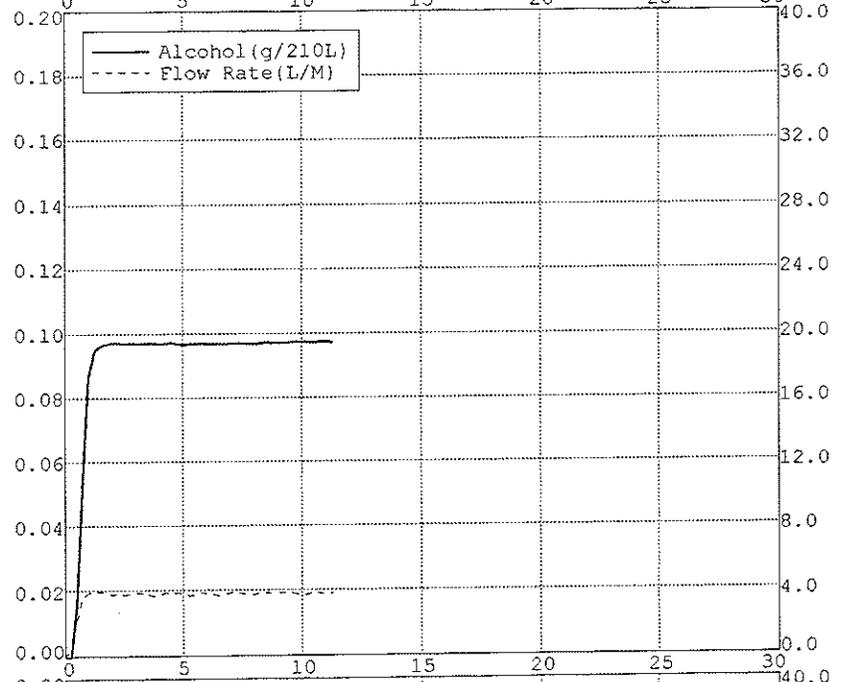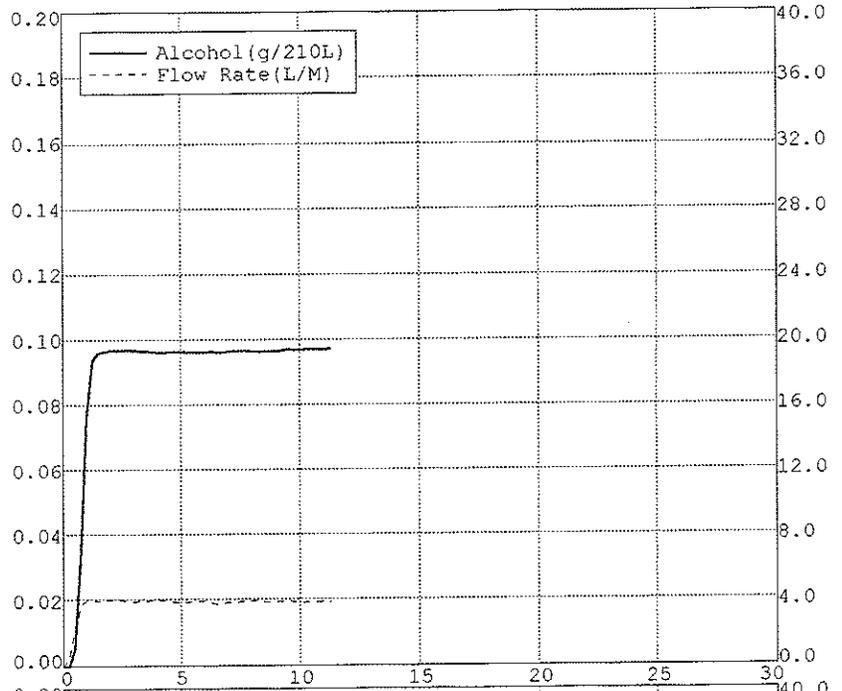

SGT *[Signature]* #757