

SOLUTION CHANGE



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/01/2025

OPERATOR NAME:
JOHN D BATEHOLTS
Permit #: 43007
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:55
INTERNAL STANDARD	VERIFIED	09:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:56
BLANK TEST	0.00	09:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:57
BLANK TEST	0.00	09:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59

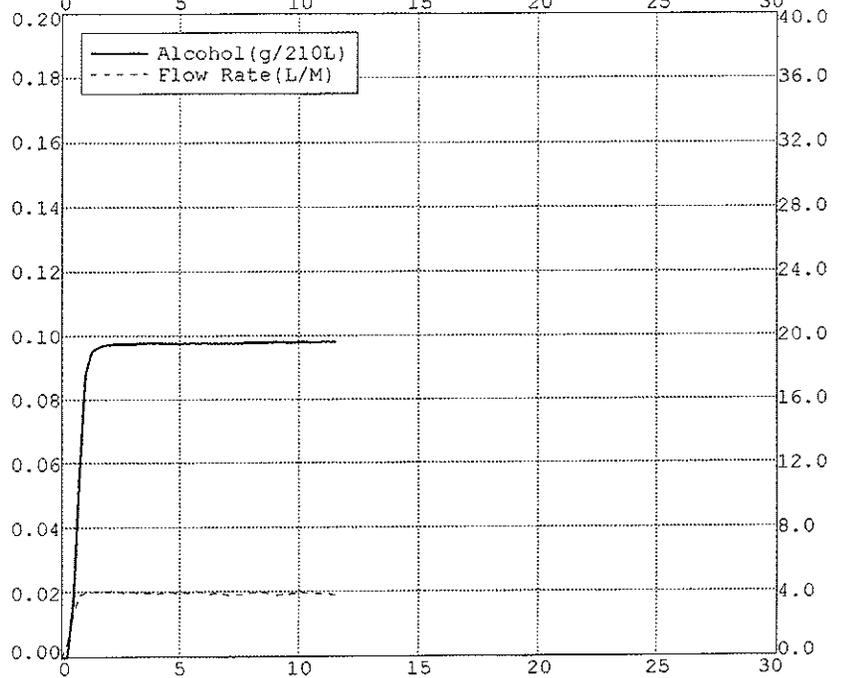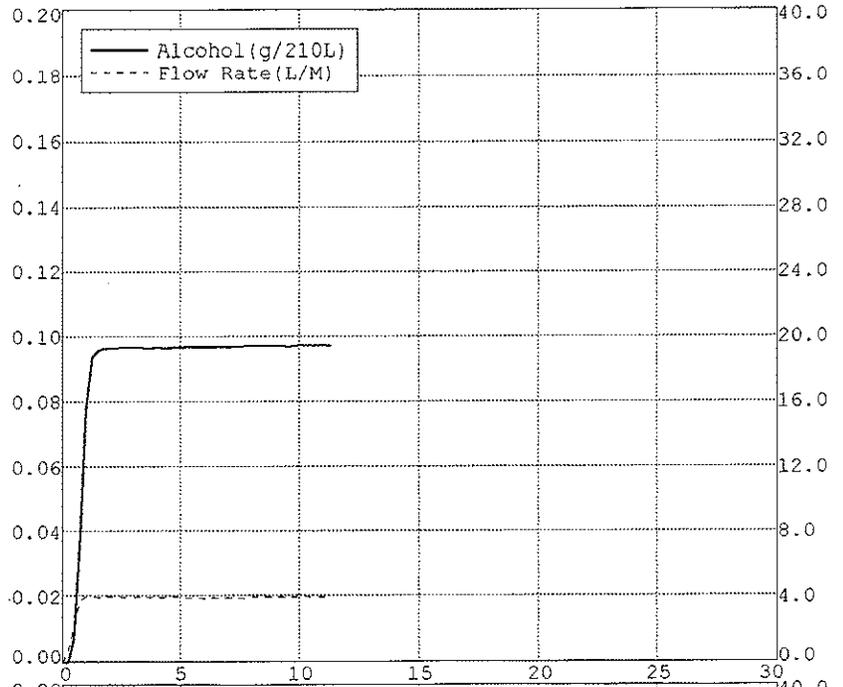

P. M. 0717