

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/26/2025

OPERATOR NAME:  
JEREMY M CRISPELL  
Permit #: 337755  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 25110

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:06
INTERNAL STANDARD	VERIFIED	09:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:07
BLANK TEST	0.00	09:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:08
BLANK TEST	0.00	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:09
BLANK TEST	0.00	09:10

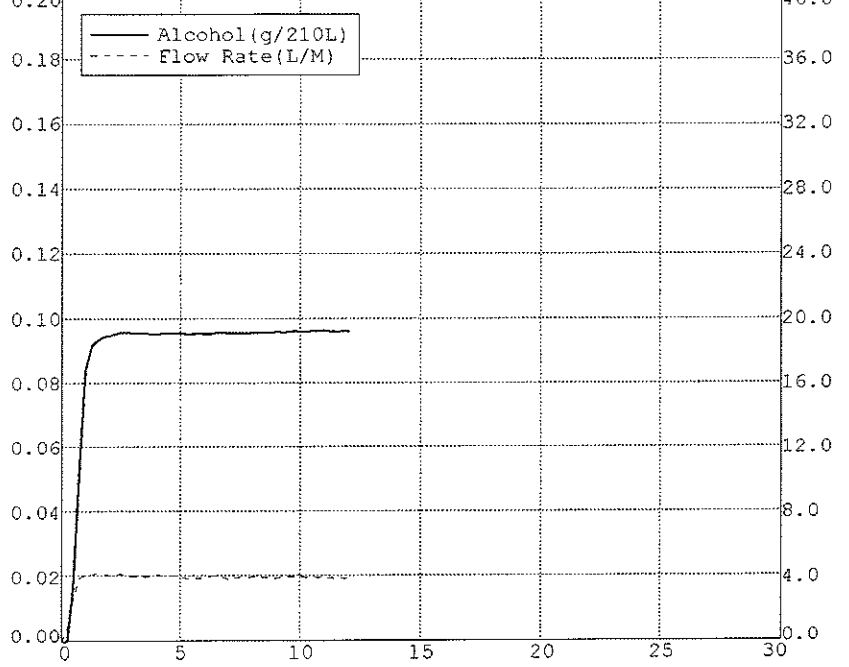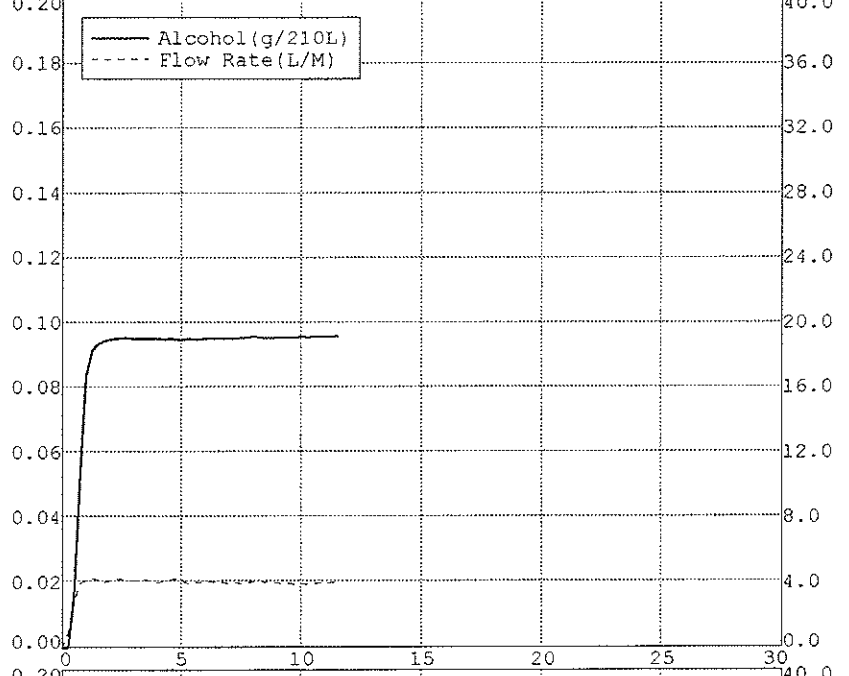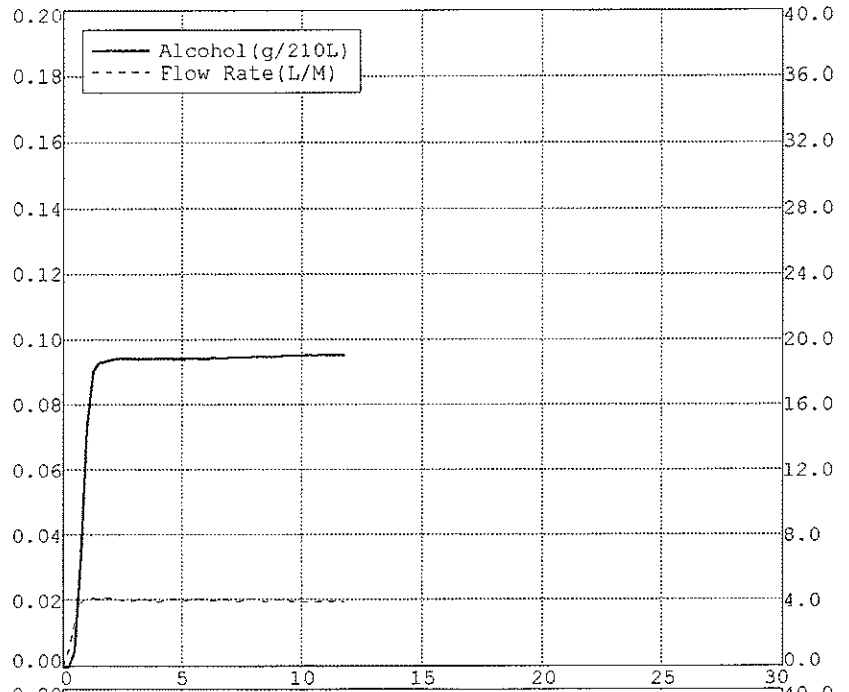

*Handwritten signature and initials*  
JMC