

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 10/17/2025

OPERATOR NAME:
ETHAN P OSTAPCZUK
Permit #: 50075
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:26
INTERNAL STANDARD	VERIFIED	02:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:26
BLANK TEST	0.00	02:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:27
BLANK TEST	0.00	02:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:28
BLANK TEST	0.00	02:29

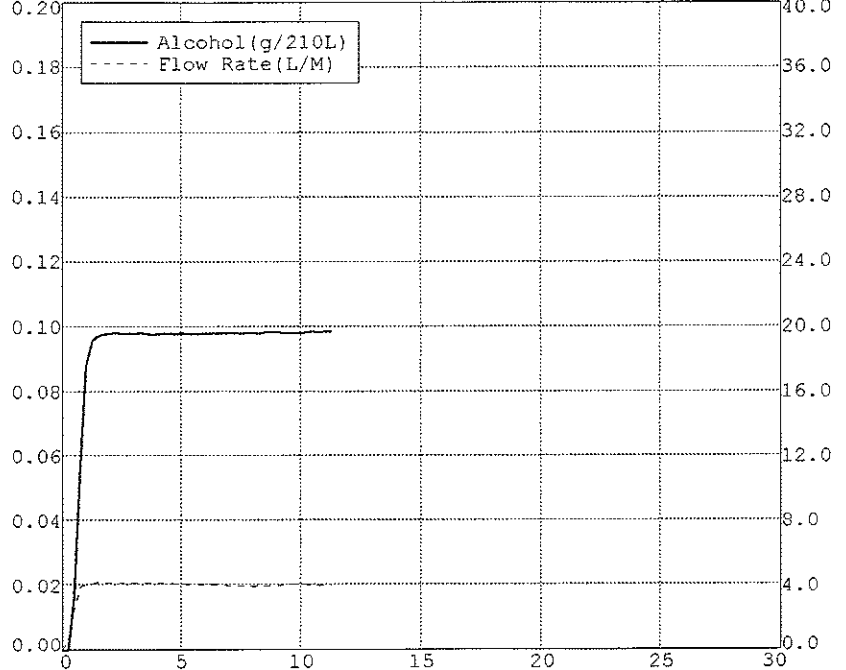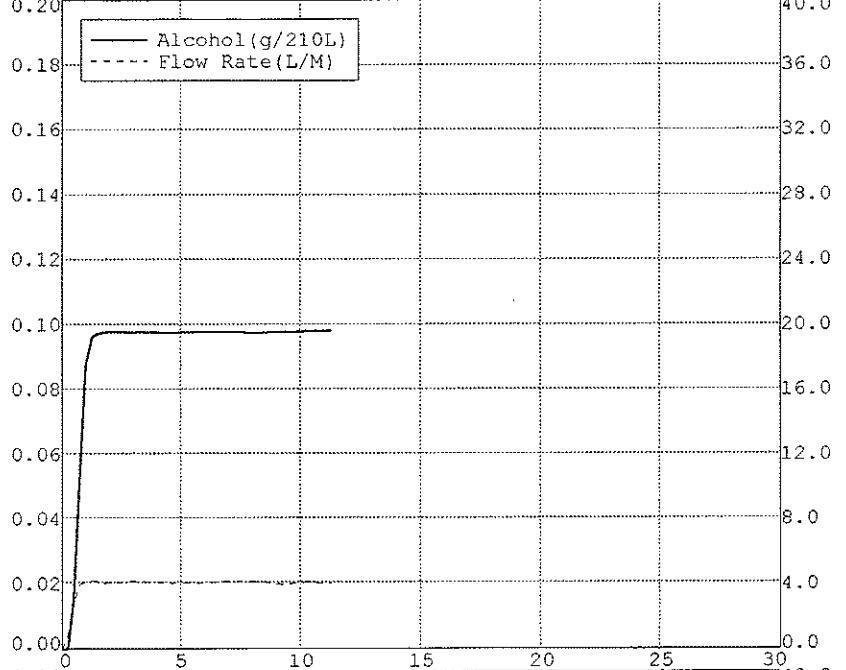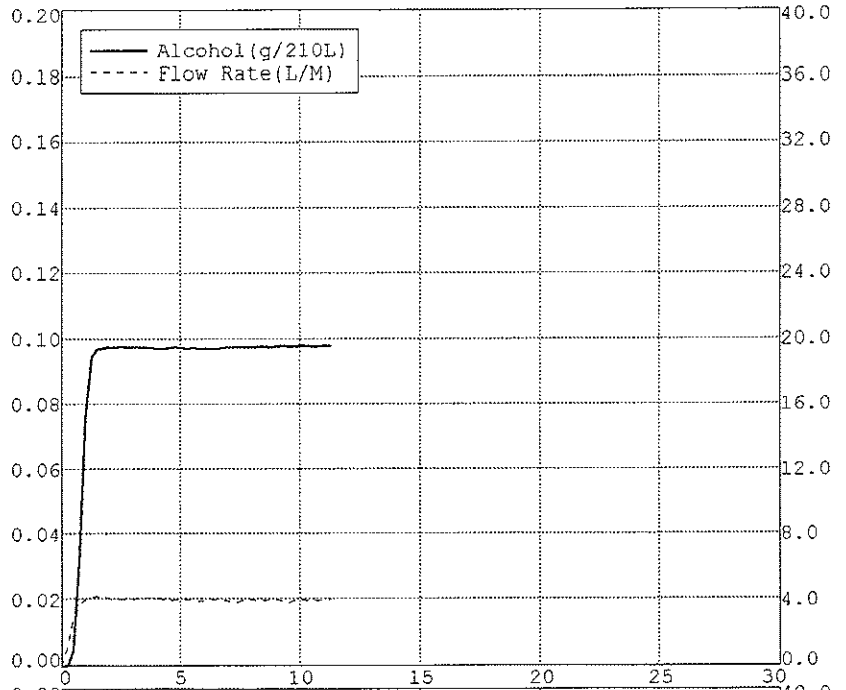

E. P. Ostapczuk #152