

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/18/2025

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:12
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16

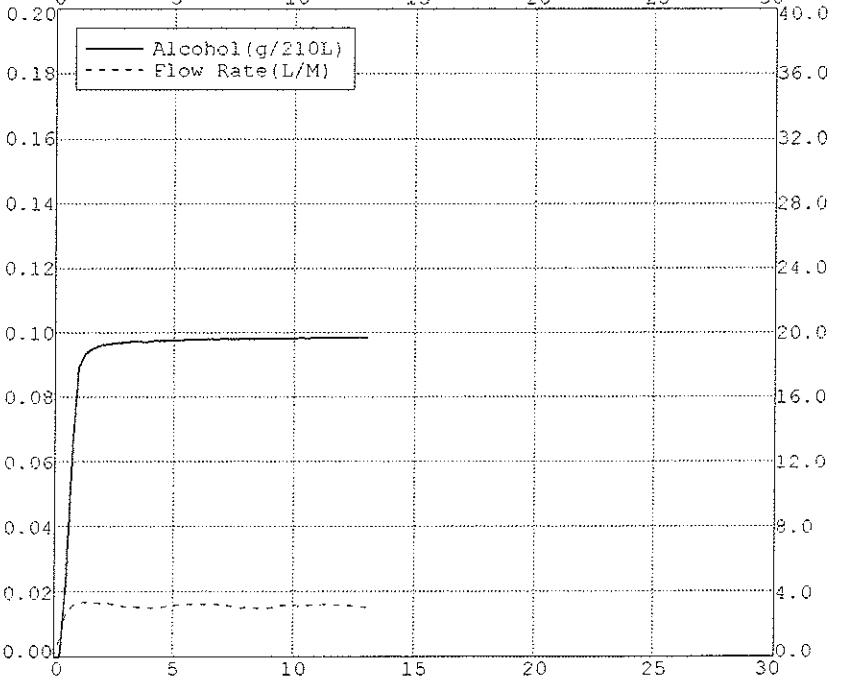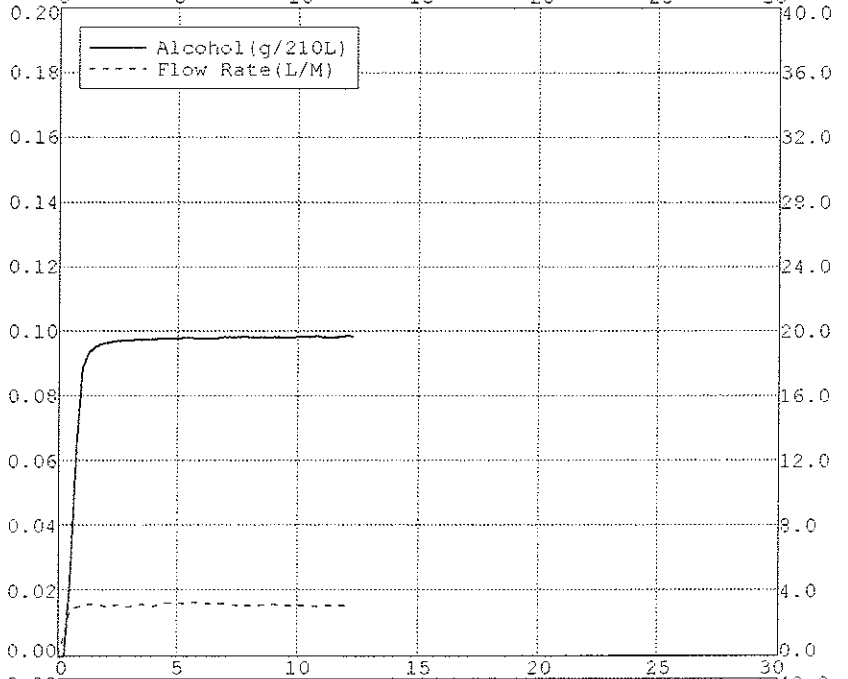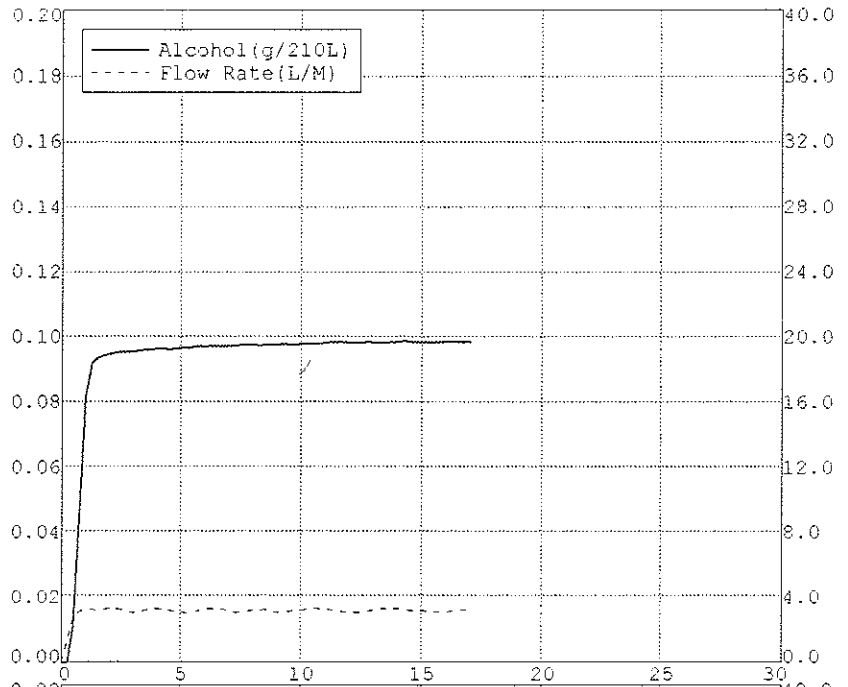

Sgt Michael A Campbell #157