

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/21/2025

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:03
INTERNAL STANDARD	VERIFIED	06:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:04
BLANK TEST	0.00	06:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:05
BLANK TEST	0.00	06:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:06
BLANK TEST	0.00	06:07

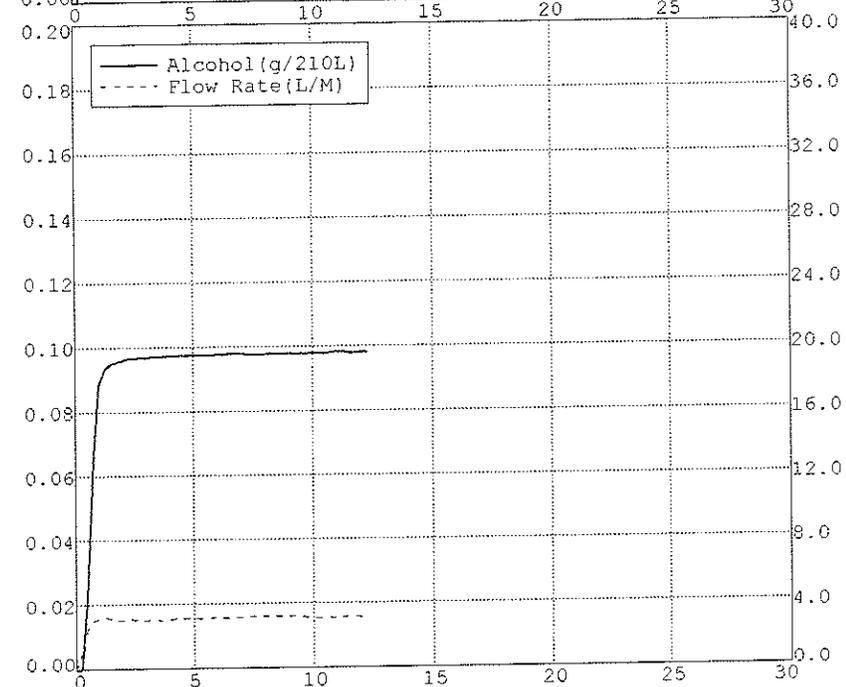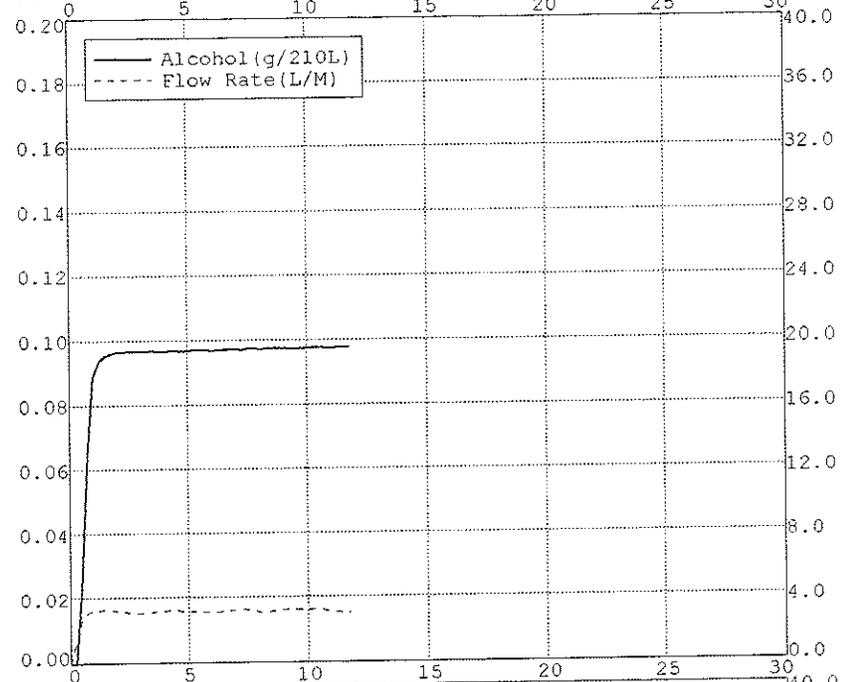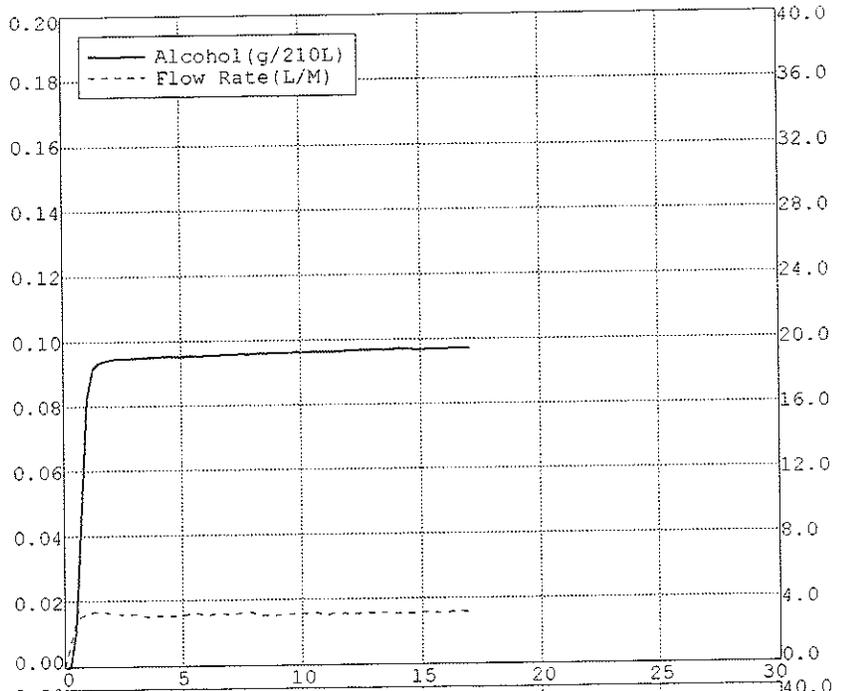

Signature #157