

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 04/04/2025

OPERATOR NAME:  
MICHAEL A CAMPBELL  
Permit #: 42422  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:16
INTERNAL STANDARD	VERIFIED	16:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:16
BLANK TEST	0.00	16:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:17
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:19
BLANK TEST	0.00	16:19

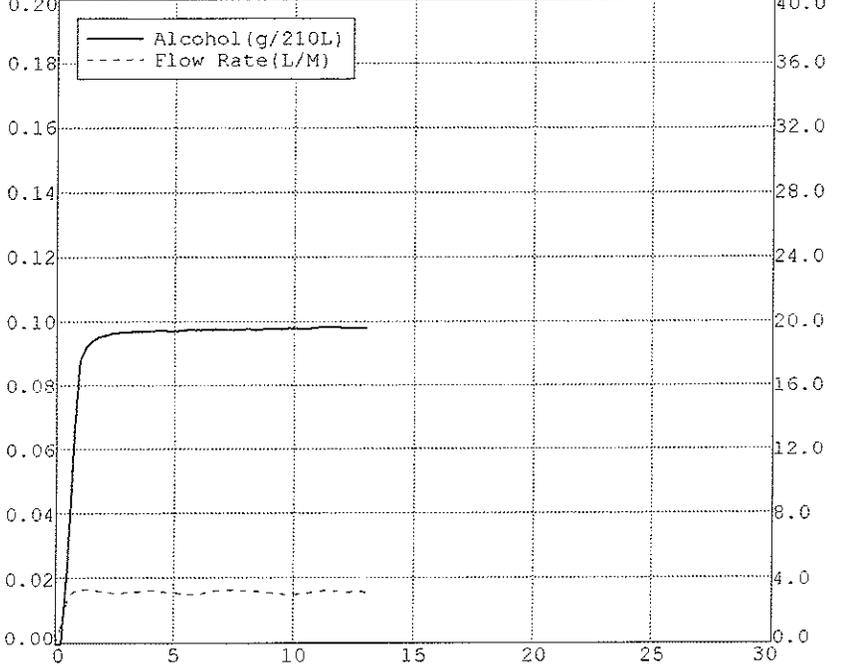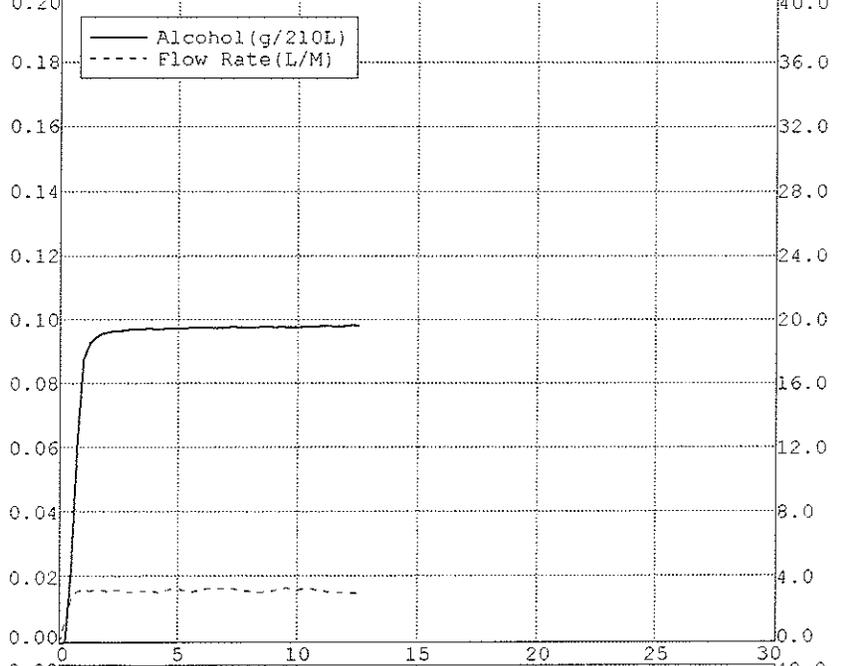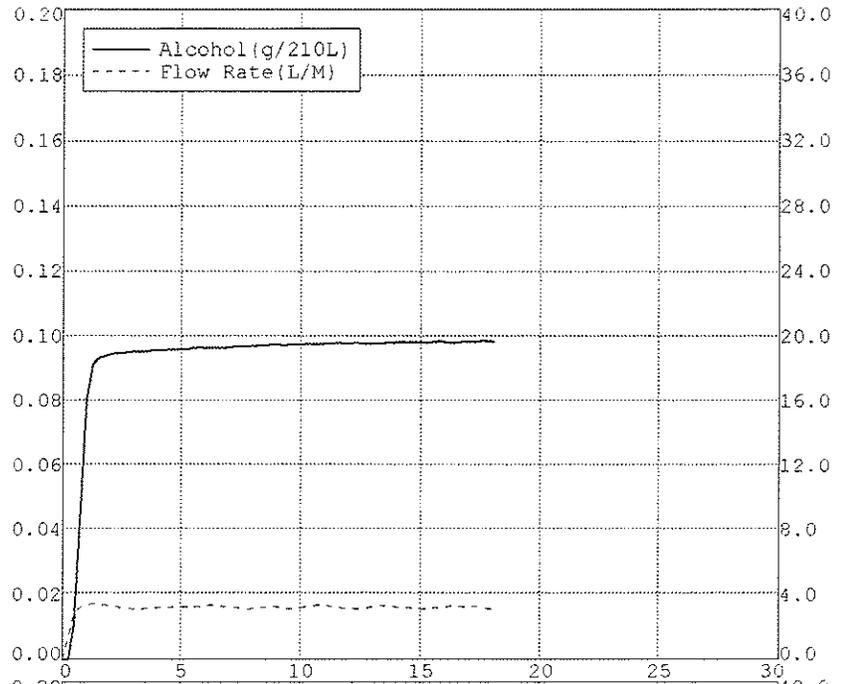

*Signature* 4/7