

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/26/2025

OPERATOR NAME:  
JEREMY M CRISPELL  
Permit #: 51155  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 10:22 |
| INTERNAL STANDARD       | VERIFIED | 10:22 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 10:22 |
| BLANK TEST              | 0.00     | 10:23 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 10:24 |
| BLANK TEST              | 0.00     | 10:24 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 10:25 |
| BLANK TEST              | 0.00     | 10:26 |

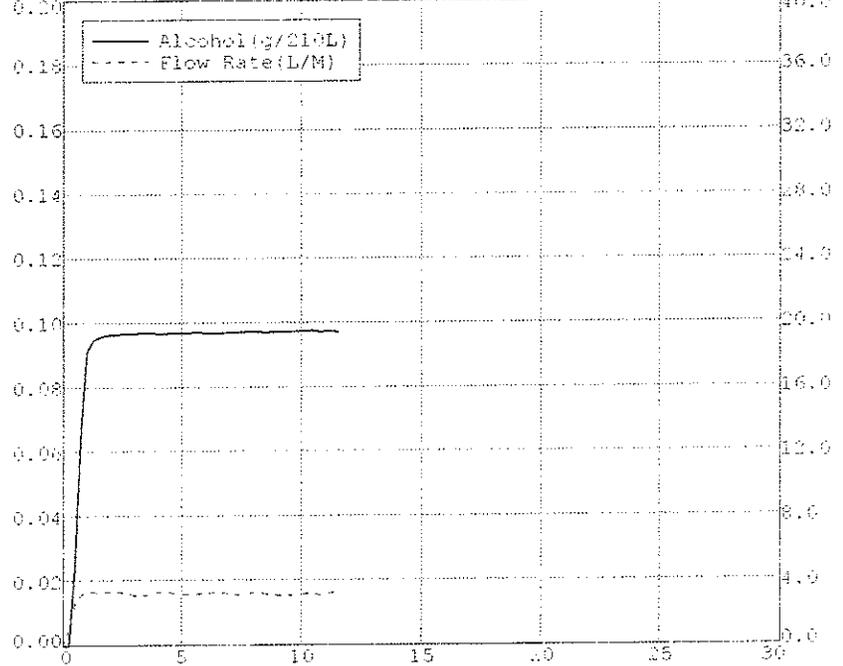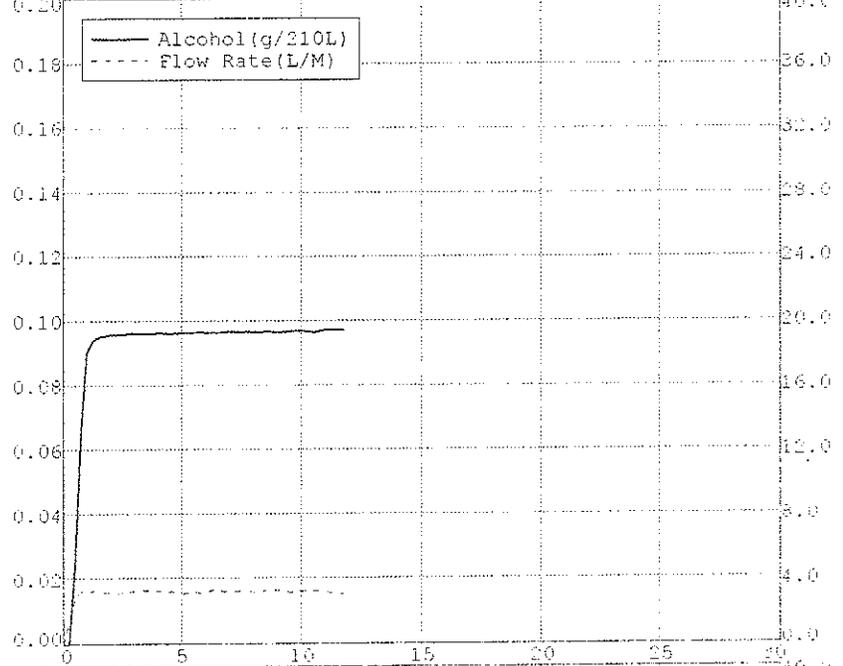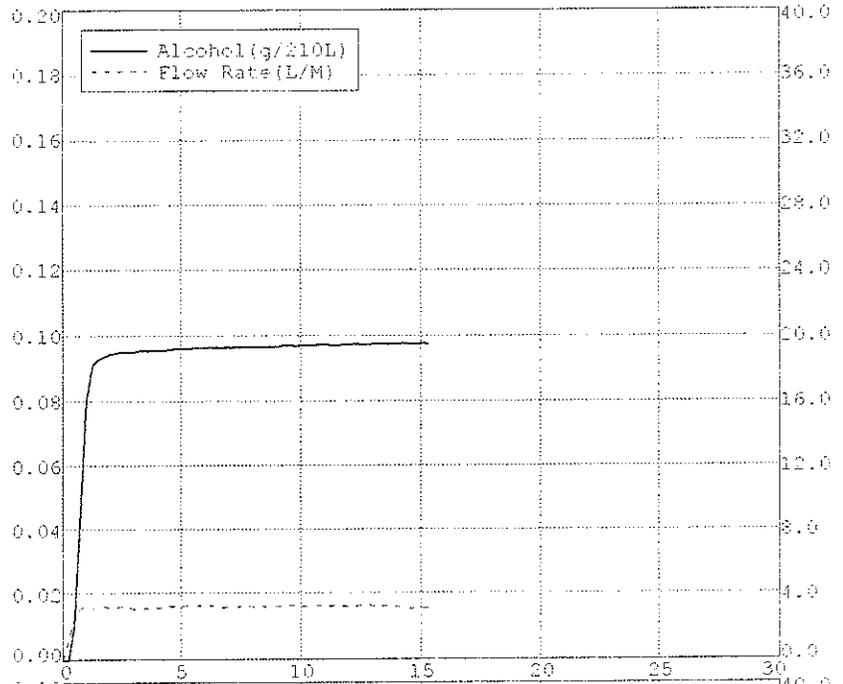

*Handwritten signature: J. M. Crispell*