

SUPERVISOR TEST



WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 10/24/2025

OPERATOR NAME:  
MICHAEL A BAKER  
Permit #: 49901  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:21
INTERNAL STANDARD	VERIFIED	13:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:22
BLANK TEST	0.00	13:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:23
BLANK TEST	0.00	13:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:24
BLANK TEST	0.00	13:25

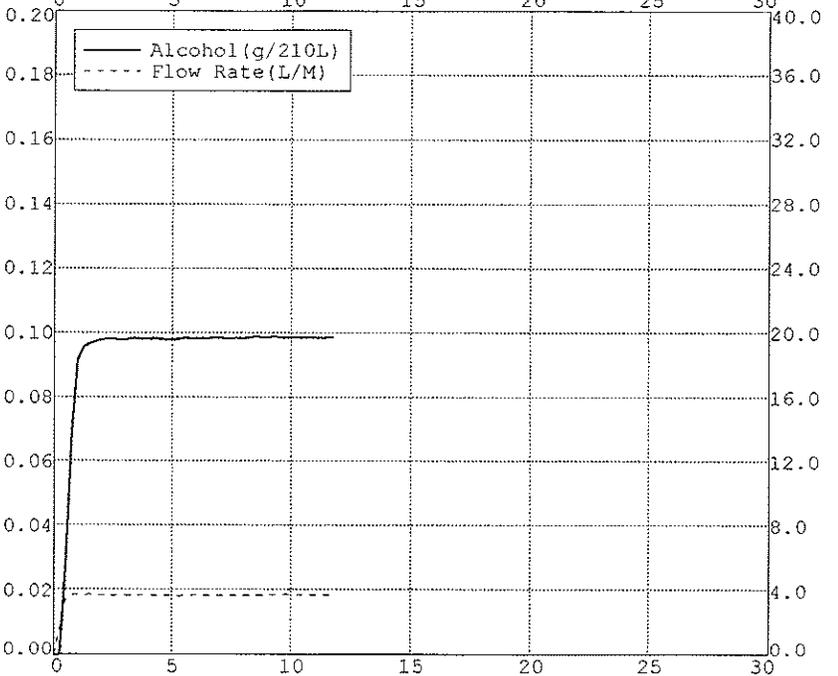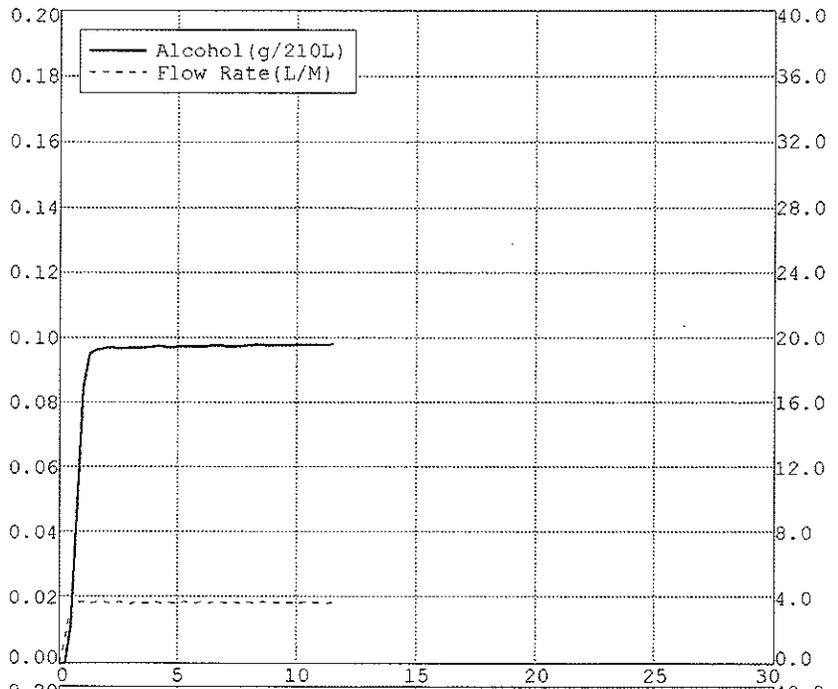

*13/10/2025 148*