

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/16/2026

OPERATOR NAME:  
RYAN C SCHROECK  
Permit #: 41316  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 25330

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:18
INTERNAL STANDARD	VERIFIED	07:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:19
BLANK TEST	0.00	07:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:20
BLANK TEST	0.00	07:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:21
BLANK TEST	0.00	07:22

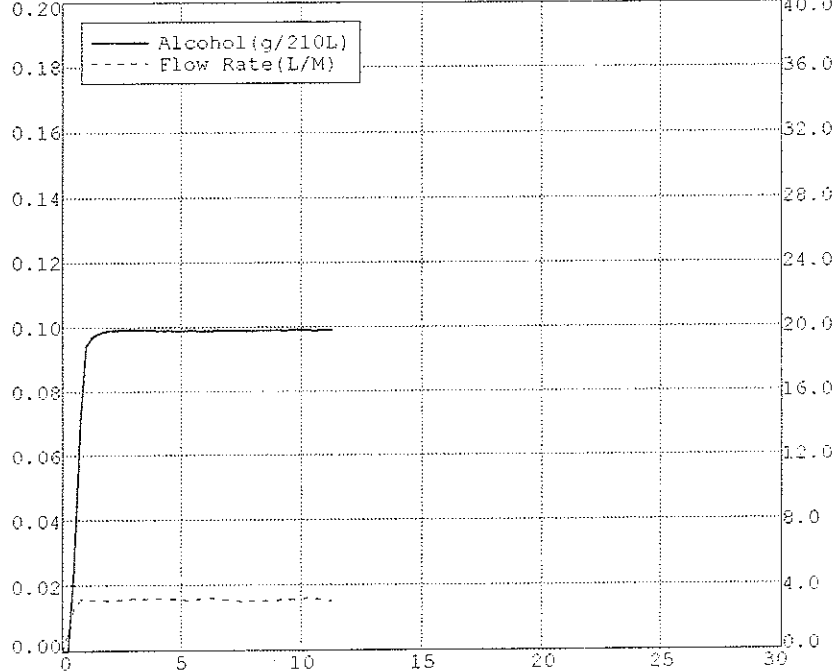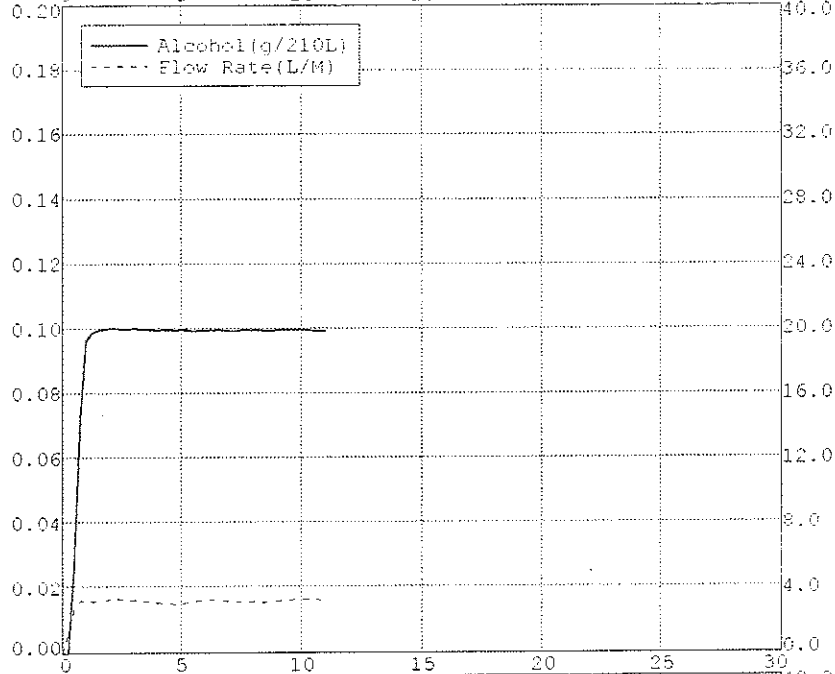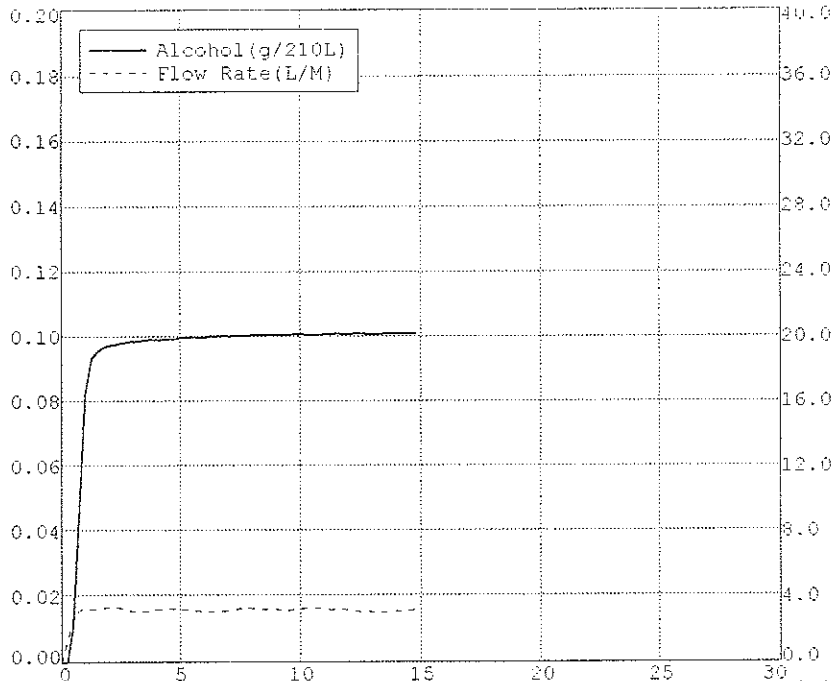

*POA 704*