



STATE OF NEW YORK  
 DIVISION OF CRIMINAL JUSTICE SERVICES  
 Alfred E. Smith State Office Bldg.  
 80 South Swan Street  
 Albany, New York 12210  
<http://criminaljustice.ny.gov>

**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
 MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Matthew J. Slater, Associate Training Technician, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 106206, performed on March 14, 2014 by Office of Public Safety employee Michael J. Hess, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

State of New York  
 County of Albany  
 Sworn to before me  
 On March 19, 2014

Matthew J. Slater  
 Associate Training Technician (Police)  
 Office of Public Safety

Notary Public, State of New York  
 Commission Expires 8/2/17

JAN A. NEAR  
 Notary Public  
 State of New York  
 Reg No. 01NE6028897  
 Qualified in Columbia County  
 Commission Expires 8/2/17

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Serial Number: 106206

Date: March 14, 2014

Reference Solution Lot Number: 13320

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.0 degrees centigrade
2	0.099 %	34.0 degrees centigrade
3	0.099 %	34.0 degrees centigrade
4	0.099 %	34.0 degrees centigrade


I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 106206, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:

Reviewed by:


  
\_\_\_\_\_  
Michael J. Hess  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 16080

  
\_\_\_\_\_  
Lisa A. Lee  
Highway Safety Equipment Technical Supervisor  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Warren County Sheriff's Office**  
**Manufacturer: NAT'L PATENT ANALYTICAL SYS**  
**Model: DATAMASTER DMT**  
**Serial Number: 106206**  
**Date: March 14, 2014**

1. General Appearance and condition of this device -----: N/A
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: OK
5. System cycles through all modes -----: OK
6. Record any repairs made to this instrument and list services provided: RAN COMMUNICATION, DIAGNOSTIC AND SUPERVISOR TESTS, VERIFIED CALIBRATION

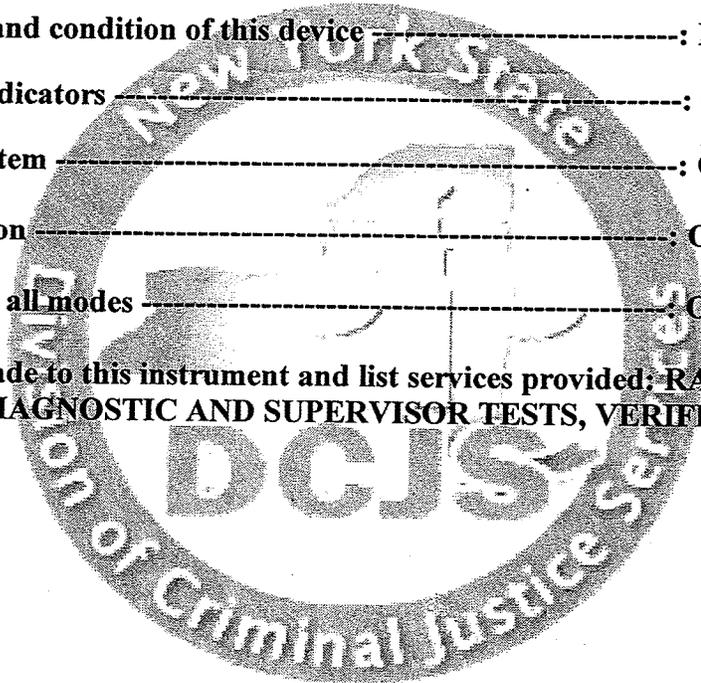

Performed by:

Reviewed by:

  
\_\_\_\_\_  
**Michael J. Hess**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 16080**

  
\_\_\_\_\_  
**Lisa A. Lee**  
**Highway Safety Equipment Technical Supervisor**  
**Breath Analysis Technical Supervisor**