



STATE OF NEW YORK  
DIVISION OF CRIMINAL JUSTICE SERVICES

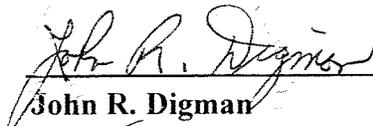
Alfred E. Smith State Office Bldg.  
80 South Swan Street  
Albany, New York 12210  
<http://criminaljustice.ny.gov>

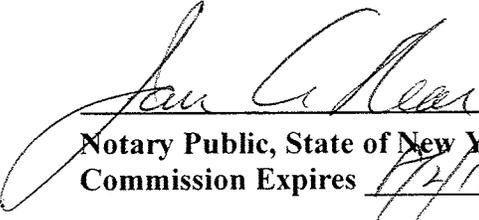
**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, John R. Digman, Special Programs Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the copies annexed hereto are exact photocopies of original records of the Office of Public Safety which are in my possession, custody and control.

I further certify that the original records of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 106206, performed on April 03, 2014 by Office of Public Safety employee Frank Sgarlata, of which the annexed are photocopies, were made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such records were made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it was the regular course of the Office of Public Safety's business to make such records at the time such inspection/ maintenance/calibration was performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

State of New York  
County of Albany  
Sworn to before me  
On April 07, 2014

  
\_\_\_\_\_  
John R. Digman  
Special Programs Supervisor  
Office of Public Safety

  
\_\_\_\_\_  
Notary Public, State of New York  
Commission Expires 4/4/17

JAN A. NEAR  
Notary Public  
State of New York  
Exp. No. 01N06028897  
Qualified in Columbia County  
Commission Expires 4/4/17

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Warren County Sheriff's Office  
 Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT  
 Date: April 03, 2014 Serial Number: 106206

Reference Solution Lot Number: 13211  
 Reference Solution Standard: 0.10% at 34.0degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.01 degrees centigrade
2	0.099 %	34.02 degrees centigrade
3	0.099 %	34.01 degrees centigrade
4	0.099 %	34.00 degrees centigrade

Reference Solution Lot Number: 13251  
 Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.077 %	34.01 degrees centigrade
2	0.078 %	34.02 degrees centigrade
3	0.077 %	34.00 degrees centigrade
4	0.077 %	34.01 degrees centigrade

Reference Solution Lot Number: 13110  
 Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

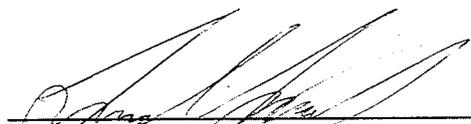
Test No	Test Result	Simulator Temperature
1	0.174 %	34.01 degrees centigrade
2	0.174 %	34.01 degrees centigrade
3	0.174 %	34.01 degrees centigrade
4	0.174 %	34.00 degrees centigrade

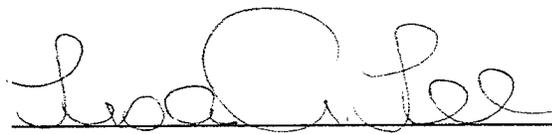
I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 106206, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:

Reviewed by:

  
 Frank Sgarlata  
 Highway Safety Equipment Technician  
 Breath Analysis Operator Permit # 36297

  
 Lisa A. Lee  
 Highway Safety Equipment Technical Supervisor  
 Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Warren County Sheriff's Office**  
**Manufacturer: NAT'L PATENT ANALYTICAL SYS**  
**Model: DATAMASTER DMT**  
**Serial Number: 106206**  
**Date: April 03, 2014**

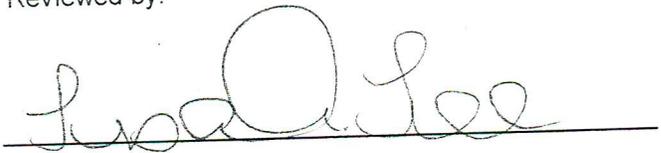
- 1. General Appearance and condition of this device -----: **LOW READINGS.**
- 2. Check controls and indicators -----: **OK**
- 3. Check breath flow system -----: **OK**
- 4. Check printer operation -----: **OK**
- 5. System cycles through all modes -----: **OK**
- 6. Record any repairs made to this instrument and list services provided: **REPLACED SAPPLE CHAMBER. CALIBRATED INSTRUMENT. RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS. CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. VERIFIED CALIBRATION.**

Performed by:



**Frank Sgarlata**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 36297**

Reviewed by:



**Lisa A. Lee**  
**Highway Safety Equipment Technical Supervisor**  
**Breath Analysis Technical Supervisor**