

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:22
INTERNAL STANDARD	VERIFIED	18:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:23
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:25
BLANK TEST	0.00	18:26

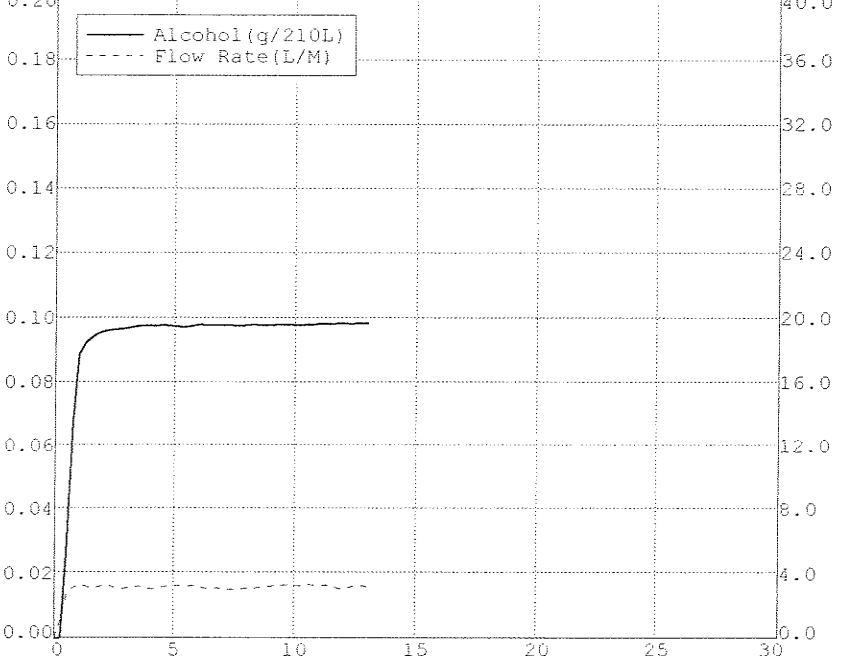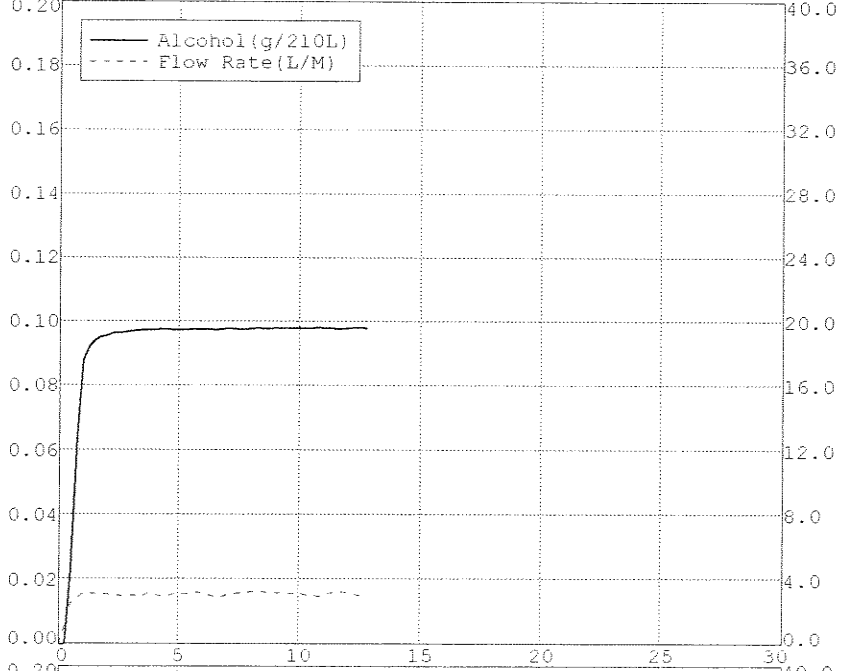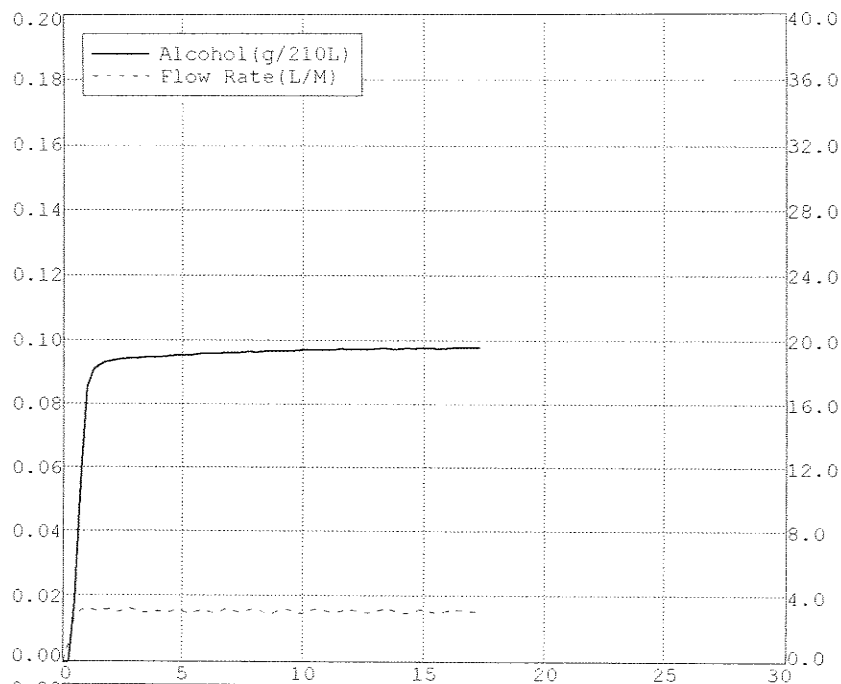

Charles B. Geisler #24