

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/27/2026

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:16
INTERNAL STANDARD	VERIFIED	20:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:16
BLANK TEST	0.00	20:17
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:18
BLANK TEST	0.00	20:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:19
BLANK TEST	0.00	20:20

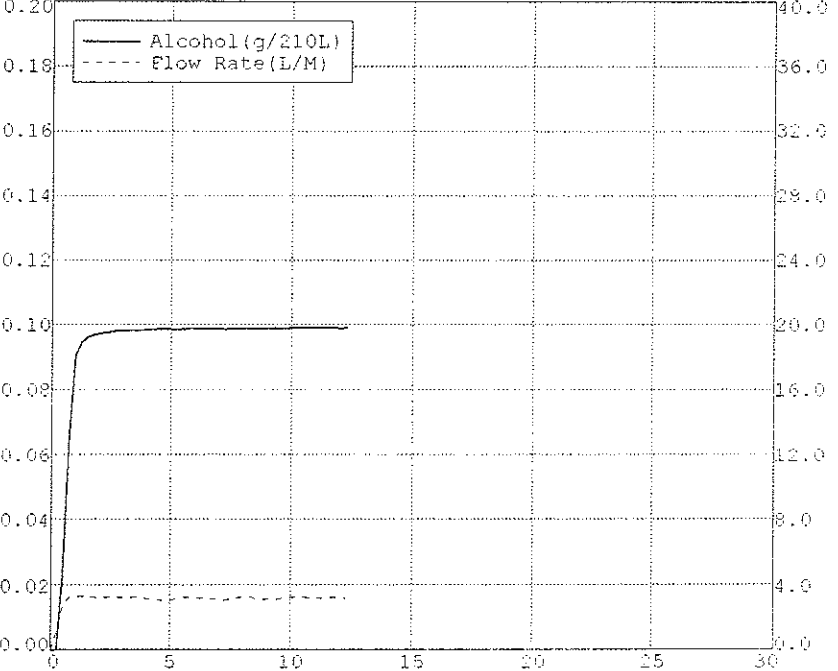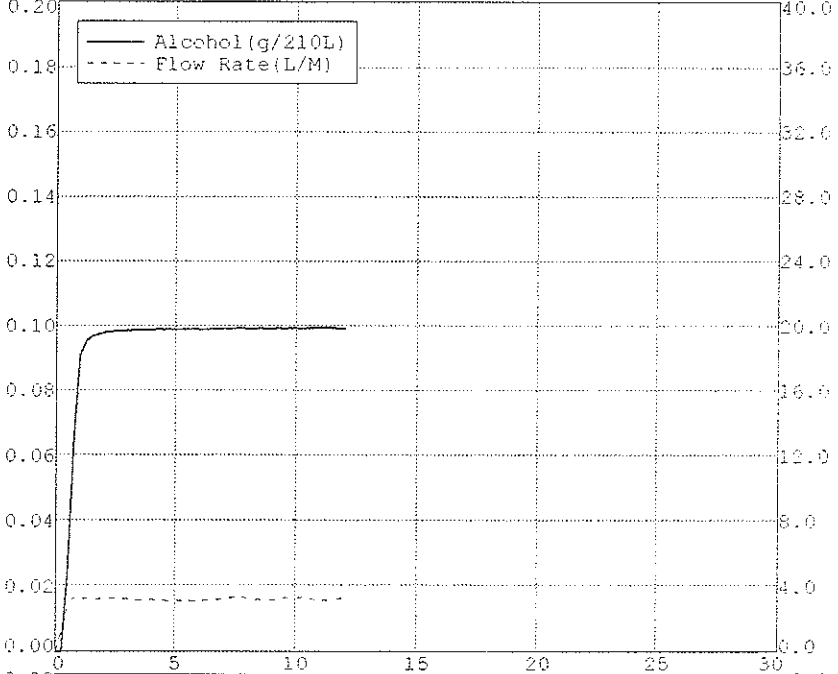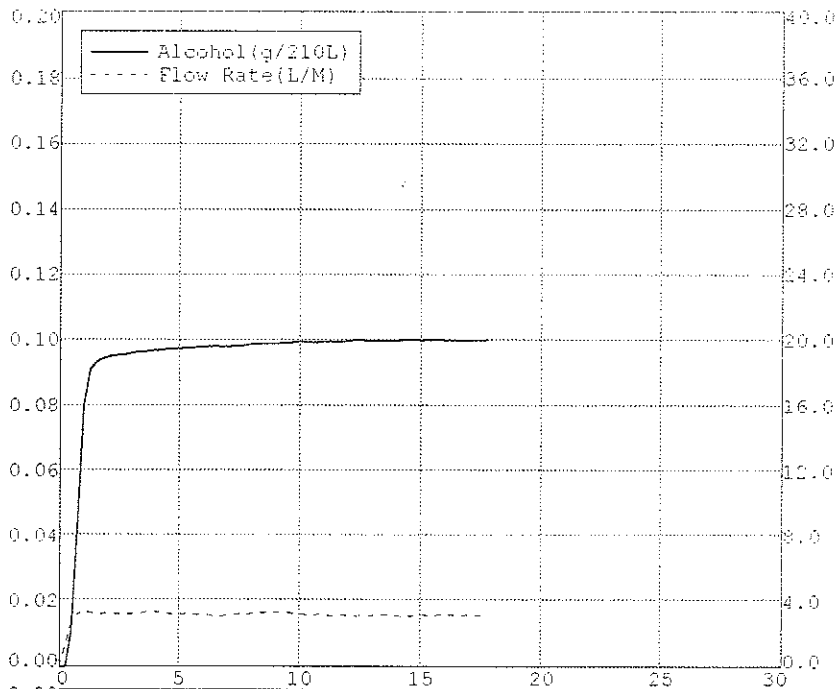

SGT *[Signature]* 757