

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/10/2026

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:30
INTERNAL STANDARD	VERIFIED	19:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:30
BLANK TEST	0.00	19:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:32
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:33
BLANK TEST	0.00	19:34

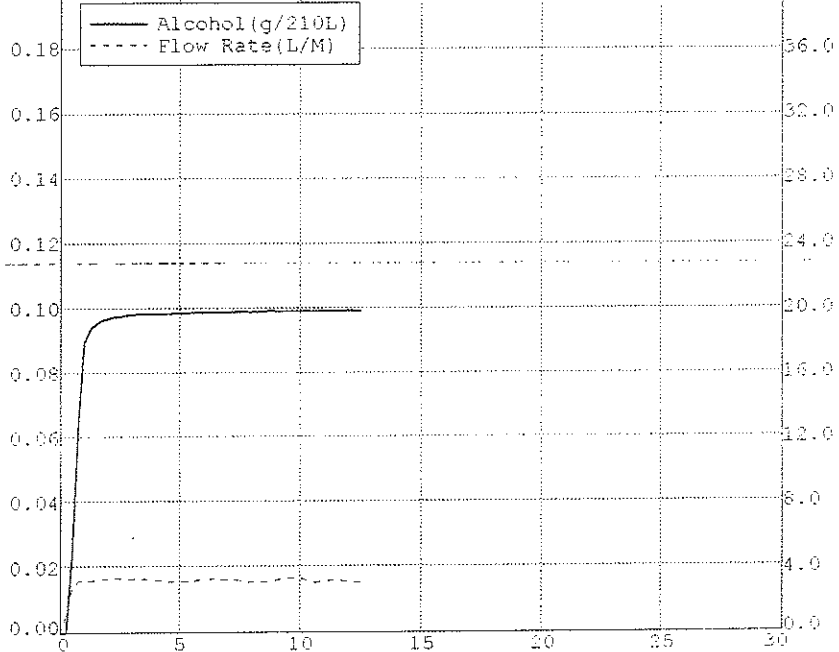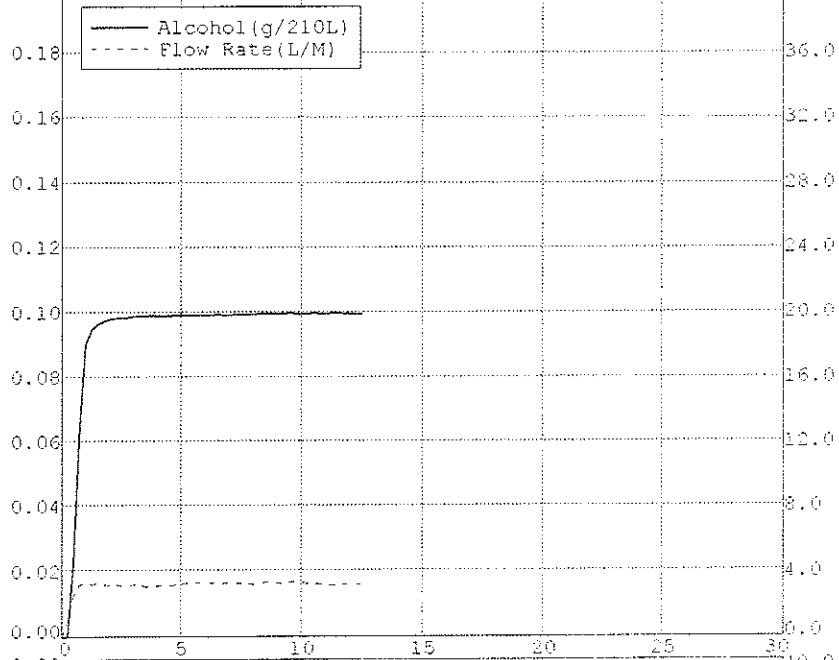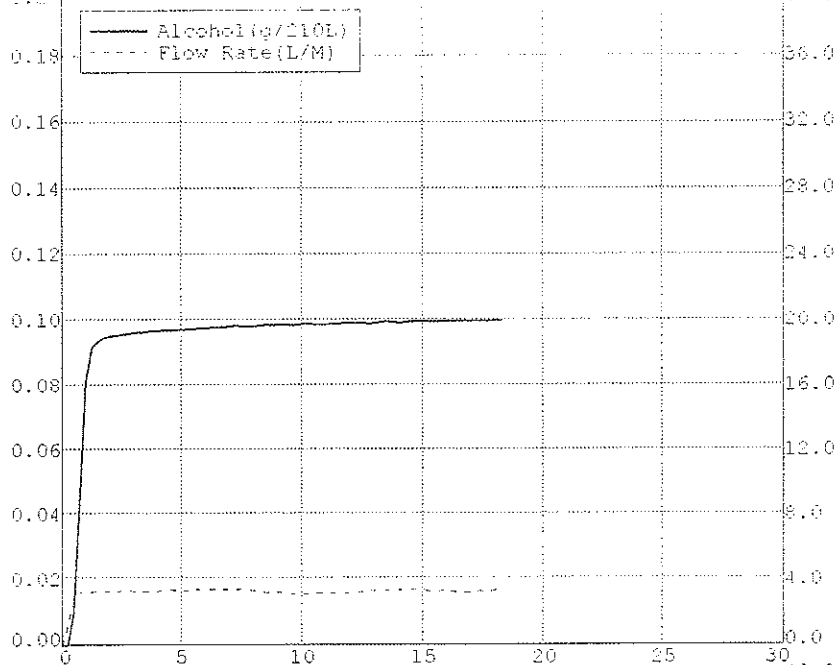

SET *[Signature]* #757